

Effect of artificial tears on dynamic optical quality in patients with dry eye disease

Zhenyu Wei

Beijing Institute of Ophthalmology, Beijing Tongren Eye Center, Beijing Tongren Hospital, Capital Medical University, Beijing Key Laboratory of Ophthalmology and Visual Sciences <https://orcid.org/0000-0001-5072-1883>

Yuandong Su

Beijing Tongren Hospital

Guanyu Su

Beijing Tongren Hospital

Christophe Baudouin

Quinze-Vingts National Ophthalmology Hospital

Antoine Labbé

INSERM

Qingfeng Liang (✉ lqflucky@163.com)

Capital Medical University <https://orcid.org/0000-0003-0000-3167>

Research article

Keywords: Objective scatter index, Tear film, Artificial tear, Dry eye

Posted Date: October 28th, 2020

DOI: <https://doi.org/10.21203/rs.3.rs-21773/v2>

License:   This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Version of Record: A version of this preprint was published at BMC Ophthalmology on February 10th, 2022. See the published version at <https://doi.org/10.1186/s12886-022-02280-7>.

Abstract

Background : In clinical practice, fluctuating vision or decreased quality of vision is a common complaint in dry eye patients. Our study was designed to investigate the change in dynamic optical quality in dry eye patients after the use of artificial tears.

Methods : Fifty-nine patients with dry eye disease (DED) and 31 healthy age- and sex-matched control subjects were included in this prospective case-control study. Clinical evaluation of the ocular surface included Ocular Surface Disease Index (OSDI), tear film break-up time (TBUT), lipid layer thickness (LLT), and Schirmer I test. DED patients were divided into two groups, mild (31 patients) and severe (28 patients). The optical quality of the tear film was measured with the Optical Quality Analysis System (OQAS) using the mean objective scatter index (mean OSI), standard deviation of objective scatter index (SD-OSI) and modulation transfer function cut-off (MTF cut-off). After baseline examinations, one drop of artificial tears (ATs, carboxymethylcellulose ophthalmic solution, 0.5%) was instilled in both eyes, and optical quality parameters were measured again at 5 and 30 minutes following application of ATs.

Results: At baseline, the mean OSI was higher in the DED group (0.95 ± 0.54) than in controls (0.54 ± 0.23 , $P < 0.001$). The SD-OSI was also significantly increased in DED patients (0.44 ± 0.71) compared to control subjects (0.12 ± 0.06 , $P = 0.003$). Five minutes after AT instillation, mean OSI and SD-OSI decreased significantly in severe DED patients ($P = 0.044$; $P = 0.018$), remained unchanged in mild DED patients, and increased in the control group ($P = 0.019$; $P < 0.001$). Thirty minutes after AT instillation, no significant difference in optical quality parameters was observed among the three groups.

Conclusion : The effect of ATs on optical quality in patients with DED may differ according to the severity of the disease. Measurement of optical quality might be a promising tool to evaluate the effects of various ATs and possibly individualize treatment in DED patients.

Background

Dry eye disease (DED) is a multifactorial disease of the ocular surface, characterized by an unstable tear film associated with symptoms of ocular surface irritation and visual impairment ^[1]. In addition to its nutritive and mechanical roles on the ocular surface, the tear film can mask irregularities of the corneal epithelium, and, consequently, it is a central component of the refractive system of the eye. Break-up of the precorneal tear film can cause irregular astigmatism in excess of 1 diopter ^[2]. In clinical practice, fluctuating vision or decreased quality of vision are common complaints in DED patients. Several studies ^[3-8] have shown that DED patients may experience transient increases in higher-order aberrations (HOA) and objective scatter index (OSI). A previous study by our group also demonstrated that OSI fluctuations were significantly increased in eyes with DED, and the degree of fluctuations was correlated with the severity of the DED ^[4]. Habay *et al.* showed similar results, with both the mean value and standard deviation of the OSI significantly decreased in severe dry eye patients ^[9].

Artificial tears (ATs), as standard first-line therapy, are typically used for DED patients, especially for aqueous deficient dry eye. Water-retentive polymers such as carboxymethylcellulose (CMC) have long been incorporated in AT formulations to supplement the aqueous, maintain and/or restore the stability of the tear film, and protect the ocular surface^[10]. Although ATs decrease ocular surface symptoms in DED patients, some patients complain of transient blurry vision or decreased visual acuity after AT use. Consequently, several studies evaluating optical quality after instilling artificial tear drops have been performed, but the results have been controversial. Some studies^[11] have reported that visual quality, as reflected by higher order aberrations (HOA), deteriorates after instilling artificial tear drops, while some studies have revealed that visual quality improves and is sustained for some time after instillation^[12]. Several reasons might explain these conflicting results, including non-objective methods of evaluation or differing severities of DED. Consequently, in the present study, we used the double pass Optical Quality Analysis System (OQAS) to evaluate the visual quality of DED patients with differing severities and normal controls after the use of 0.5% CMC ATs. The goal was to evaluate the effect of ATs on optical quality in DED patients.

Methods

Subjects

This study was conducted at the Beijing Tongren Hospital with the approval of the hospital's Medical Ethics Committee (TREC-2017-KY021). All subjects were informed of the goals of the study, and their consent was obtained in accordance with the declaration of Helsinki. A total of 59 DED patients (36 women and 23 men; mean age 36.05 ± 12.56 years; range 18–72 years) were consecutively recruited from July 2018 to August 2019. In keeping with the consensus report by the International Dry Eye Workshop (2007)^[13], the inclusion criteria for the DED group were as follows: (1) age > 18 years; (2) Ocular Surface Disease Index (OSDI) score greater than 12; (3) tear film break-up time (TBUT) less than 10 seconds; (4) Schirmer I test at 5 minutes less than 10 mm. According to the severity-grading scheme of the 2007 Workshop^[13], DED patients were divided into two groups (mild and severe). The severe DED group (28 patients) included patients with Schirmer I test ≤ 5 mm. The mild DED group (31 patients) consisted of patients with Schirmer I test between 5 and 10 mm. Thirty-one age- and gender-matched control subjects (21 women and 10 men; mean age 38.13 ± 13.79 years, range 18–67 years) were also recruited, with Schirmer I test results exceeding 10 mm at 5 minutes, TBUT above 10 seconds and an OSDI score below 13. The exclusion criteria for both groups were as follows: (1) age < 18 years; (2) subjects unable to complete the questionnaire or understand the procedures; (3) best corrected visual acuity less than 20/20; (4) presence of ocular or systemic disease or the use of topical or systemic medications that may affect the ocular surface, and (5) previous history of eye surgery or contact lens wear.

Clinical Evaluation

Each subject underwent a quantification of ocular surface symptoms with the Ocular Surface Disease Index (OSDI) questionnaire (range 0-100) ^[14]. Optical quality and ocular surface examinations were then performed in the following order: double-pass optical quality analysis, lipid layer thickness measurement (LLT), TBUT and Schirmer I test.

The lipid layer thickness was measured with the Lipiview II® device (Tear science, Morrisville, NC, USA). The interferometric color unit (ICU) value reflected the local LLT with 1 ICU equivalent to 1 nm of lipid layer thickness. TBUT was measured using sterile fluorescein strips impregnated with 0.6 mg fluorescein sodium (Alcon Laboratories, St. Louis, MO, USA). After applying 50 µL of normal saline solution to the paper strip, it was touched to the inferior fornix. The interval between a complete blink and the appearance of the first dry spot was noted. TBUT was measured 3 times, and the mean calculated. The Schirmer's test was performed without anesthesia after having the patient's eyes closed for 5 minutes.

Objective scatter index measurement

The Optical Quality Analysis System (OQAS-II, Visiometrics, Tarrasa, Spain), was used to evaluate aberrations and intraocular scatter with the 2 following parameters: objective scatter index (OSI) and modulation transfer function cut-off (MTF cut-off). The OSI is defined as the ratio between the integrated light in the peripheral ring and the central peak of the double-pass (DP) image. It represents the impact of aberration and scattering on the DP image. The MTF cut-off is the cut-off point on the x-axis of the MTF curve, which can be directly calculated from the point spread function. The MTF cut-off reflects the highest spatial frequencies that can be distinguished by patients' eyes at which the MTF reaches the lowest contrast of 1%. The subjects were tested with their best correction and instructed to blink normally during the double-pass analysis. The "Tear Film Analysis" program of the commercially available OQAS device was used to record dynamic changes in OSI values. This program consisted of a 20-second examination with OSI measurement every 0.5 sec, providing a graph showing the change in OSI over time (Figure 1). The pupil size was set at 7 mm to cover the majority of the tear film. After measurement, the mean value and standard deviation of the 20-second OSI was recorded as "mean OSI" and "SD OSI," respectively.

After baseline examination, the effect of artificial tears was studied on the following day. One drop of artificial tears (carboxymethylcellulose ophthalmic solution 0.5%, Refresh Plus, Allergan Pharmaceuticals, Ireland) was instilled in both eyes. Five and thirty minutes after application, the OQAS examinations were performed again in all subjects. The difference between the mean OSI at baseline and at 5 and 30 minutes (OSI_{5min} , OSI_{30min}) were analyzed, and the relationship between OSI and DED severity was evaluated.

Statistical analysis

Statistical analysis was performed with SPSS for Windows, version 22.0 (SPSS Inc., Chicago, IL, USA). For each subject, both eyes were tested, and the right eye was selected for analysis. All values were expressed as mean \pm SD. The normality of the data was analyzed using the Shapiro-Wilk test. The normal

data were compared before and after treatment with the paired *t*-test, and the non-normal data were used for the paired rank-sum test. A Bonferroni correction of multiple comparisons was included. The generalized estimation equation was used to compare the repeated measurement data at each time point and within each treatment group. The Spearman correlation test was used to evaluate the correlation between the visual quality parameters and dry eye clinical tests. A $P < 0.05$ was considered statistically significant.

Results

Subject clinical characteristics

There was no difference with respect to gender ($P=0.342$) or age ($P=0.847$) between the DED (mild and severe group) and control groups. Regarding ocular surface symptoms, DED patients had more symptoms (OSDI score: mild group 24.04 ± 5.22 , severe group 52.66 ± 14.10) than normal controls (8.67 ± 3.29) (all $P < 0.001$). In addition, the TBUT in the mild (4.05 ± 1.08 sec) and severe (3.17 ± 0.99 sec) DED groups was significantly less than in normal controls (11.84 ± 3.12 sec), ($P < 0.001$). Compared to control subjects (16.26 ± 4.98 mm), the Schirmer I test was lower in the mild (8.48 ± 2.74 mm, $P < 0.001$) and severe group (3.83 ± 1.25 mm; $P < 0.001$). The mild and severe DED patients had significantly lower LLT (59.29 ± 15.53 nm, $P=0.015$; 54.14 ± 16.84 nm, $P=0.001$) compared to normal controls (70.81 ± 19.33 nm). However, no statistical difference in LLT was observed between the two DED groups ($P=0.223$) (Table 1).

Optical quality analysis at baseline

The results of the optical quality examinations at baseline showed that the MTF cut-off value in the mild (32.11 ± 11.16 , $P=0.002$) and severe (32.84 ± 11.84 , $P=0.004$) groups was significantly decreased compared to normal subjects (40.96 ± 9.07). The mean OSI was significantly increased in the severe group (1.05 ± 0.65 , $P < 0.001$) compared to normal subjects (0.54 ± 0.23). This difference was not significant in the mild group (0.83 ± 0.38 , $P=0.020$). There was no statistical difference between the mild and severe DED groups for the mean OSI ($P=0.060$). The SD OSI value in the severe DED group (0.47 ± 0.72) was significantly higher than in normal subjects (0.12 ± 0.06) ($P=0.004$), and there was no significant difference between the mild (0.41 ± 0.69) and control groups ($P=0.024$) (Figure 2).

Changes in optical quality after AT application

Five minutes after AT instillation, the mean and SD of the OSI increased significantly in the control group, from 0.54 ± 0.23 and 0.12 ± 0.06 at baseline to 0.69 ± 0.27 and 0.20 ± 0.10 , respectively ($P=0.019$ and $P < 0.001$). In the mild group, the mean OSI (1.00 ± 0.48) and the SD OSI (0.13 ± 0.05) did not change significantly compared to the baseline results (0.83 ± 0.38 , $P=0.155$; 0.40 ± 0.70 , $P=0.066$). In the severe group, both the mean OSI (0.78 ± 0.36 vs. 1.05 ± 0.65 , $P=0.044$) and the SD OSI (0.15 ± 0.08 vs. 0.47 ± 0.72 , $P=0.018$) decreased significantly at 5 minutes after AT application. Inversely, compared to baseline values, the parameters of mean and SD OSI had no significant difference at 30 minutes after AT instillation in any of the groups (Figure 3).

Correlation between change in optical quality and clinical tests

Within the DED groups, there were significant negative correlations between TBUT and mean OSI ($r = -0.329$, $P=0.011$), and TBUT and SD-OSI ($r = -0.330$, $P=0.011$). TBUT was also positively correlated with the $\Delta\text{OSI}_{5\text{min}}$ ($r = 0.261$, $P=0.045$). Similarly to the TBUT, the Schirmer I test was negatively correlated with the mean OSI ($r = -0.251$, $P=0.050$) and SD-OSI ($r = -0.349$, $P=0.007$) and positively correlated with the $\Delta\text{OSI}_{5\text{min}}$ ($r = 0.457$, $P=0.000$) (Table 2).

Discussion

Blurred vision and visual fluctuations are significant complaints in DED patients. Previous studies have found that the visual disturbances in DED are related to the unstable tear film [3-5]. As a component of the refractive system of the eye, the tear film covers the ocular surface and corrects for irregularities in the corneal epithelium [2]. The optical quality of the tear film has been considered as a parameter for evaluation of the stability of the tear film and the severity of DED [15-17]. Similarly to previous studies, our study showed that optical quality parameters (MTF cut-off, mean OSI and SD-OSI) were changed in DED patients and these changes are correlated to DED severity.

When considering the effects of ATs on DED patients, the results of previous studies evaluating quality of vision have been controversial [18-24]. In 1993, Rieger *et al.* [22] suggested that ATs could improve contrast sensitivity for severe DED patients. Misaki *et al.* [23] detected changes in visual acuity with different concentrations of ATs and found no significant difference in mild patients' visual acuity 5 minutes after AT application. However, these two studies only focused on the changes in visual quality a few minutes after AT instillation. Tung *et al.* [24] presented differing results, with a decrease in visual quality 5 minutes after AT instillation, but they did not analyze different DED severity groups. In the present study, 5 minutes after instillation, the severe and mild dry eye and normal subjects showed differing results. An increase in optical quality was observed in the severe group, there was no change in the mild group, and significant degradation of optical quality was shown in normal subjects. The improvement in optical quality may be related to the severity of tear volume deficiency. In the severe group, in whom the Schirmer I test was less than 5 mm, artificial tears can quickly restore the aqueous layer and the optical role of the tear film on the ocular surface. In the mild group, a trend toward improvement in the SD OSI was observed, but these changes were not significant.

In our study, the OSI mean and SD showed no significant difference at 30 minutes after AT instillation in any of the groups. These findings are consistent with previous studies showing a rapid return of tear film biomarkers to baseline after AT instillation. In a study evaluating the tear meniscus depth and height by optical coherence tomography (OCT), Carracedo *et al.* [29] found no statistically significant difference in tear volume and stability between baseline and 20 minutes after AT instillation. The same results were observed by Napoli *et al.* [30]. In their study, 20 minutes after instillation of ATs, the tear film thickness and

tear meniscus volume returned to baseline values in all groups. Moreover, in the study by Koh, there was a correlation between wavefront error and tear meniscus height ^[31].

In our study, the OSI mean and SD values increased after AT application in the control group, which is consistent with previous studies ^[24, 32]. Our first hypothesis is that the volume of ATs might dilute the original tear film in normal patients and change the biochemical properties such as viscosity or refractive index. This may lead to tear film instability and subsequently to an increased tear meniscus, as revealed by Shizuka *et al.* ^[32]. In DED patients, the key optical problem is tear deficiency on the ocular surface. Consequently, it might be replenished by ATs, with resultant improvement in visual quality. Nevertheless, in the present study, after AT instillation, the improved mean OSI in severe DED patients was more obvious than in normal subjects at baseline. Consequently, the hypothesis of the lubricant-only role of ATs might not completely explain this result. Another hypothesis could be the role of osmolarity. The cell membrane of corneal epithelial cells is a semi-permeable membrane allowing fluid transport within the intercellular space depending on particle concentration. With increased evaporation, the tear volume decreases, and the osmolarity of the tear film increases. Previous studies have shown that tear osmolarity in mild and severe DED patients is significantly increased (approximately 315 mOsm/L and 336 mOsm/L, respectively) compared to normal controls (302 mOsm/L) ^[33]. Most types of ATs for DED treatment have been hypo-osmolar ^[34]. Similarly, the AT used in the present study (Refresh Plus) has an osmolarity of 294 ± 2 mOsm/L, lower than that of the tear film ^[34]. Therefore, five minutes after instillation, the ocular surface osmolarity may be equilibrated to a new lower level. In DED patients, the tear volume was replenished and tear film osmolarity decreased to the normal level, leading to an increase in tear film stability and visual quality. The effect of ATs on normal subjects might be different. The osmolarity of the tear film might decrease due to dilution by hypotonic ATs. Following the osmotic pressure gradient, the corneal epithelial cells might become edematous, characterized by swelling of the epithelial cells and distension of the intercellular spaces ^[35], causing light to be scattered and visual quality to be decreased.

Although there are several limitations to the present study, including the use of only one type of ATs and the lack of characterization of the type of DED (i.e. meibomian gland dysfunction vs. aqueous deficiency), we showed that the effect of ocular lubricants on visual quality may vary according to the severity of DED. Another limitation is interference of the examinations, especially Schirmer's testing, with the tear film. To minimize the impact of prior testing, we added a control group and examined the effect of artificial tears on the following day.

The objective evaluation of optical quality with the OQAS seems to be an interesting clinical parameter that can be easily associated with and compared to the classic clinical signs used in DED. It may be a promising tool in evaluating the effects of various ATs and possibly individualizing treatment in DED patients, avoiding those preparations which cause the most blurred vision and favoring those which improve quality of vision over a longer period.

Conclusions

In summary, our data indicate that optical quality may be improved significantly five minutes after AT instillation in severe DED cases, unchanged in mild DED cases, and decreased in the normal controls. For this reason, measurement of optical quality could be a promising tool to evaluate the effects of ATs in DED patients. The data support our hypothesis that the visual quality of DED patients may be influenced by AT application, and these differences may depend on the severity of DED. To make up for the lack of current research, our future studies might focus on the effect of various ATs and dynamic changes in optical quality. We might also concentrate on patients with evaporative dry eye.

Our present and future studies might eventually help DED patients individualize therapy in terms of selecting the most beneficial artificial tear. This study may also be significant to the improvement of the components and technology of artificial tears.

Abbreviations

ATs: Artificial tears; **DED:** Dry eye disease; **DP:** Double-pass; **HOA:** Higher-order aberrations; **ICU:** Interferometric color unit; **LLT:** Lipid layer thickness; **Mean OSI:** Mean Objective Scatter Index; **MTF cut-off:** Modulation transfer function cut-off; **OSDI:** Ocular Surface Disease Index; **OSI:** Objective scatter index; **OQAS:** Optical Quality Analysis System; **SD-OSI:** Standard deviation of objective scatter index; **TBUT:** Tear film break-up time; **OCT:** optical coherence tomography.

Declarations

Ethics and consent to participate

This study was conducted at the Beijing Tongren Hospital with the approval of the hospital's Medical Ethics Committee (TREC-2017-KY021). All subjects were informed of the goals of the study. In accordance with Helsinki declaration, written and verbal consent for participation in the study was obtained from all participants.

Consent for publication

Not applicable.

Availability of data and materials

The datasets used and analyzed in this study are available from the corresponding author on reasonable request.

Competing interests

The authors declare that they have no competing interests.

Funding

National Nature Science Foundation of China (81970765); Beijing Science and technology project (Z181100001918031), China. These funds were used to purchase research equipment and reagents.

Authors' contributions

ZW and YS analyzed and interpreted the data and were the major contributors in writing the manuscript. They contributed equally to this work. QL, as the corresponding author, was primarily responsible for experimental design and revision of the paper. GS and LW contributed to data acquisition and the rough draft. CB and AL made a substantial contribution to the revision of the manuscript. All authors read and approved the final manuscript.

Acknowledgements

We gratefully acknowledge the research participants who contributed immeasurably to this study.

References

1. Tsubota K, Yokoi N, Shimazaki J, et al. New Perspectives on Dry Eye Definition and Diagnosis: A Consensus Report by the Asia Dry Eye Society. *Ocul Surf* 2017, 15(1):65-76.
2. Montes-Mico R. Role of the tear film in the optical quality of the human eye. *Journal of cataract and refractive surgery* 2007, 33(9):1631-1635.
3. Kobashi H, Kamiya K, Yanome K, et al. Longitudinal assessment of optical quality and intraocular scattering using the double-pass instrument in normal eyes and eyes with short tear breakup time. *PloS one* 2013, 8(12):e82427.
4. Tan CH, Labbe A, Liang Q, et al. Dynamic change of optical quality in patients with dry eye disease. *Invest Ophthalmol Vis Sci* 2015, 56(5):2848-2854.
5. Yan Jiangbo, et al. A double-pass method of evaluating the optical quality of dry eye caused by meibomian gland dysfunction. *Chinese Journal of Optometry Ophthalmology and Visual science*. 2015, 11(17).
6. Montes-Mico R, Alio JL, Munoz G, et al. Temporal changes in optical quality of air-tear film interface at anterior cornea after blink. *Invest Ophthalmol Vis Sci* 2004, 45(6):1752-1757.
7. Li KY, Yoon G. Changes in aberrations and retinal image quality due to tear film dynamics. *Optics express* 2006, 14(25):12552-12559.
8. Montes-Mico R, Alio JL, Charman WN. Dynamic changes in the tear film in dry eyes. *Invest Ophthalmol Vis Sci* 2005, 46(5):1615-1619.
9. Habay T, Majzoub S, Perrault O, et al. Objective assessment of the functional impact of dry eye severity on the quality of vision by double-pass aberrometry. *J Fr Ophtalmol* 2014, 37(3):188-194.
10. Albarran C, Pons AM, Lorente A, et al. Influence of the tear film on optical quality of the eye. *Cont Lens Anterior Eye* 1997, 20(4):129-135.

11. Goto E, Yagi Y, Matsumoto Y, et al. Impaired functional visual acuity of dry eye patients. *Am J Ophthalmol* 2002, 133(2):181-186.
12. Montes-Mico R, Caliz A, Alio JL. Wavefront analysis of higher order aberrations in dry eye patients. *Journal of refractive surgery (Thorofare, NJ : 1995)* 2004, 20(3):243-247.
13. The definition and classification of dry eye disease: report of the Definition and Classification Subcommittee of the International Dry Eye WorkShop (2007). *Ocul Surf* 2007, 5(2):75-92.
14. Miller KL, Walt JG, Mink DR, et al. Minimal clinically important difference for the ocular surface disease index. *Archives of ophthalmology (Chicago, Ill : 1960)* 2010, 128(1):94-101.
15. Nilforoushan MR, Latkany RA, Speaker MG. Effect of artificial tears on visual acuity. *Am J Ophthalmol* 2005, 140(5):830-835.
16. Simmons PA, Vehige JG. Clinical performance of a mid-viscosity artificial tear for dry eye treatment. *Cornea* 2007, 26(3):294-302.
17. Kobashi H, Kamiya K, Igarashi A, et al. Intraocular Scattering after Instillation of Diquafosol Ophthalmic Solution. *Optom Vis Sci* 2015, 92(9):e303-309.
18. Koh S, Maeda N, Ikeda C, et al. Effect of instillation of eyedrops for dry eye on optical quality. *Invest Ophthalmol Vis Sci* 2013, 54(7):4927-4933.
19. McGinnigle S, Eperjesi F, Naroo SA. A preliminary investigation into the effects of ocular lubricants on higher order aberrations in normal and dry eye subjects. *Cont Lens Anterior Eye* 2014, 37(2):106-110.
20. Diaz-Valle D, Arriola-Villalobos P, Garcia-Vidal SE, et al. Effect of lubricating eyedrops on ocular light scattering as a measure of vision quality in patients with dry eye. *Journal of cataract and refractive surgery* 2012, 38(7):1192-1197.
21. Montes-Mico R, Cervino A, Ferrer-Blasco T, et al. Optical quality after instillation of eyedrops in dry-eye syndrome. *Journal of cataract and refractive surgery* 2010, 36(6):935-940.
22. Rieger G. Contrast sensitivity in patients with keratoconjunctivitis sicca before and after artificial tear application. *Graefes Arch Clin Exp Ophthalmol.* 1993;231(10):577–579.
23. Ishioka M, Kato N, Takano Y, et al. The quantitative detection of blurring of vision after eyedrop instillation using a functional visual acuity system. *Acta Ophthalmol.* 2009;87(5):574–575.
24. Tung CI, Kottaiyan R, Koh S, et al. Noninvasive, objective, multimodal tear dynamics evaluation of 5 over-the-counter tear drops in a randomized controlled trial. *Cornea.* 2012;31(2):108–114.
25. van den Berg TJ. To the editor: Intra- and intersession repeatability of a double-pass instrument. *Optom Vis Sci.* 2010;87(11):920–921.
26. Lee K, Sohn J, Choi JG, Chung SK. Optical quality in central serous chorioretinopathy. *Invest Ophthalmol Vis Sci.* 2014;55(12):8598–8603.
27. Lee K, Sohn J, Choi JG, Chung SK. Optical quality in central serous chorioretinopathy. *Invest Ophthalmol Vis Sci.* 2014;55(12):8598–8603.
28. Cho JH, Bae SH, Kim HK, Shin YJ. Optical Quality Assessment in Patients with Macular Diseases Using Optical Quality Analysis System. *J Clin Med.* 2019;8(6):892.

29. Carracedo G, Pastrana C, Serramito M, et al. Evaluation of tear meniscus by optical coherence tomography after different sodium hyaluronate eyedrops instillation. *Acta Ophthalmol.* 2019;97(2):e162-e169.
30. Napoli PE, Satta GM, Coronella F, et al. Spectral-domain optical coherence tomography study on dynamic changes of human tears after instillation of artificial tears. *Invest Ophthalmol Vis Sci.* 2014;55(7):4533-4540.
31. Koh S, Tung C, Aquavella J, et al. Simultaneous measurement of tear film dynamics using wavefront sensor and optical coherence tomography. *Invest Ophthalmol Vis Sci.* 2010;51(7):3441-3448.
32. Koh S, Tung CI, Inoue Y, Jhanji V. Effects of tear film dynamics on quality of vision. *Br J Ophthalmol.* 2018;102(12):1615–1620.
33. Sullivan BD, Whitmer D, Nichols KK, Tomlinson A, Foulks GN, Geerling G, Pepose JS, Kosheleff V, Porreco A, Lemp MA: An objective approach to dry eye disease severity. *Invest Ophthalmol Vis Sci* 2010, 51(12):6125-6130.
34. Bitton E, Perugino C, Charette S: Comparison of Ocular Lubricant Osmolalities. *Optom Vis Sci* 2017, 94(6):694-699.
35. Goldman JN, Kuwabara T. Histopathology of corneal edema. *Int Ophthalmol Clin* 1968, 8(3):561-579.

Tables

Table 1. Demographic information and baseline results of ocular surface tests.

	Control	Mild DED	Severe DED	Pvalue	Pvalue (subgroup comparison)		
	(31 eyes)	(28 eyes)	(31 eyes)	within groups	control vs mild	control vs severe	mild vs severe
Male	10	13	10	0.342	0.269	0.785	0.171
Female	21	15	21				
Age, y	38.13±13.79	37.71±13.43	36.35±14.40	0.847	0.982	0.678	0.564
OSDI, units	8.67±3.29	24.04±5.22	52.66±14.10	<0.001	<0.001	<0.001	<0.001
TBUT, s	11.84±3.12	4.05±1.09	3.17±0.99	0.002	<0.001	<0.001	0.024
Schirmer I, mm	16.26±4.98	8.48±2.74	3.83±1.25	<0.001	<0.001	<0.001	<0.001
LLT, nm	70.81±19.33	59.29±15.33	54.14±16.84	0.015	0.009	<0.001	0.452

Note: Data were expressed as the means ± SD. Due to multiple comparisons, the inspection level was corrected to 0.0125.

Table 2. Optical quality comparison of participants before after artificial tears application

	n	Mean OSI			SD OSI		
		Baseline	5 min	30 min	Baseline	5 min	30 min
Normal control	31	0.54±0.23	0.69±0.27	0.56±0.29	0.12±0.06	0.20±0.10	0.13±0.05
t value			-2.418	-0.338		-3.802	-0.481
P value			0.019	0.737		0.000	0.632
Mild ADDE	28	0.83±0.38	1.00±0.48	0.91±0.53	0.40±0.70	0.13±0.05	0.28±0.27
t value			-1.444	-0.597		1.966	0.848
P value			0.155	0.553		0.066	0.402
Severe ADDE	31	1.05±0.65	0.78±0.36	0.83±0.76	0.47±0.72	0.15±0.08	0.36±0.38
t value			2.073	1.214		2.508	0.752
P value			0.044	0.299		0.018	0.455

Note: Data were expressed as the means ± SD. "Mean OSI" and "SD OSI" refer to the mean value and standard deviation of the 20-second OSI.

Table 3. Statistical results of correlations between DED clinical tests and optical quality change

	OSDI	BUT	Schirmer I test	LLT
MTF cut-off				
R	0.089	0.164	-0.026	-0.114
<i>P</i>	0.505	0.216	0.843	0.399
Mean OSI				
R	-0.013	-0.329	-0.257	-0.063
<i>P</i>	0.921	0.011	0.050	0.643
SD-OSI				
r	0.056	-0.330	-0.349	-0.134
<i>P</i>	0.676	0.011	0.007	0.320
OSI_{5min}				
r	0.063	0.261	0.457	0.042
<i>P</i>	0.633	0.045	0.000	0.758
OSI_{30min}				
r	-0.093	-0.013	-0.037	0.178
<i>P</i>	0.558	0.906	0.745	0.111

Note: The MTF cut-off, mean OSI, and SD OSI values were measured at baseline. The OSI_{5min} and OSI_{30min} were defined as the difference between the mean OSI at baseline and 5 or 30 minutes after AT instillation.

Figures

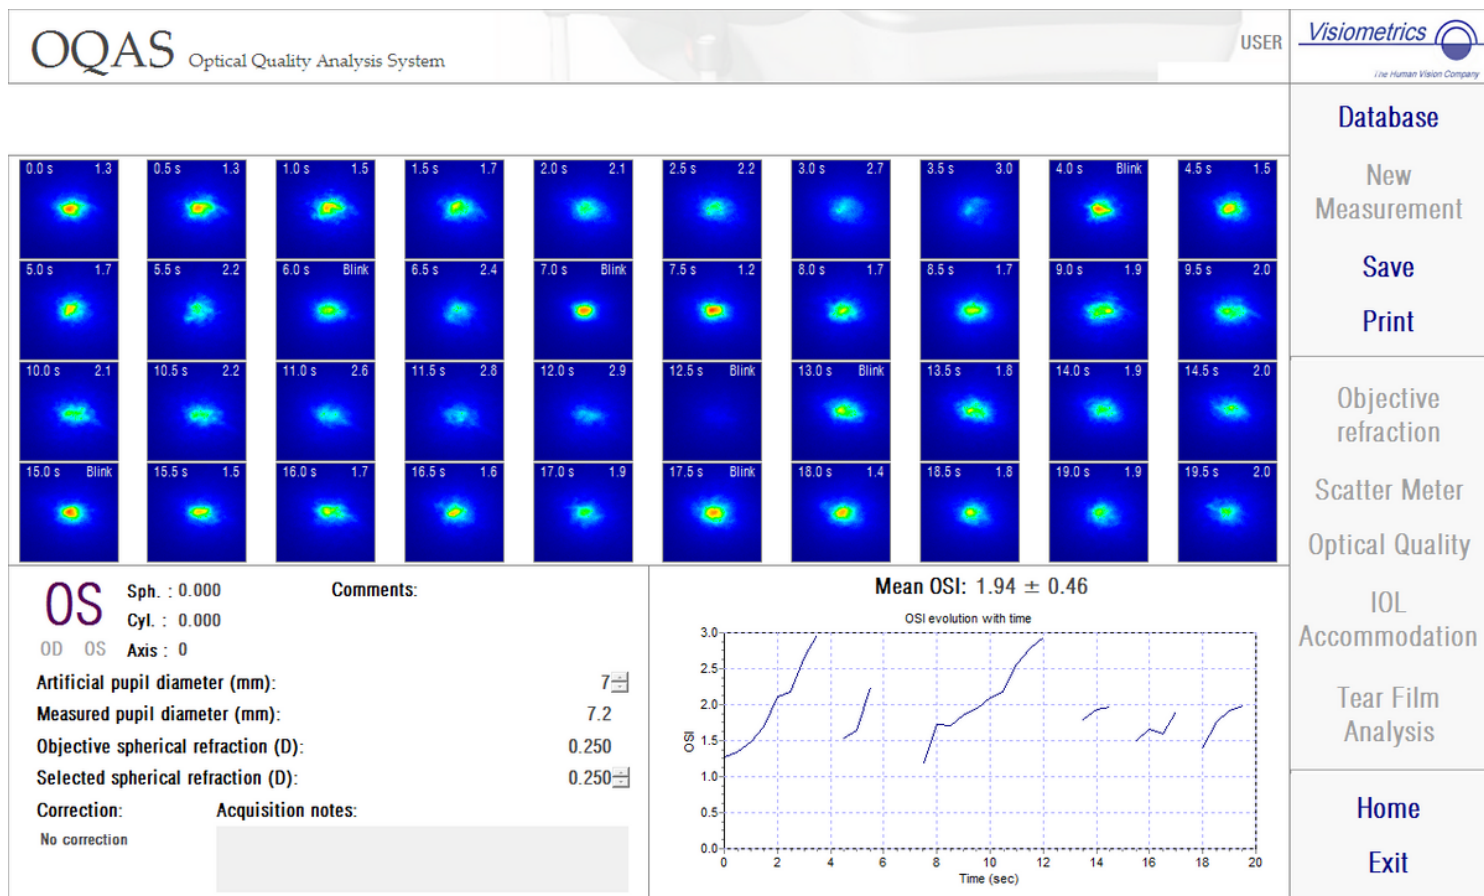


Figure 1

The “Tear Film Analysis” program of OQAS device. This device records a 20-second examination with OSI measurement every 0.5 sec, providing a graph showing the change in OSI over time

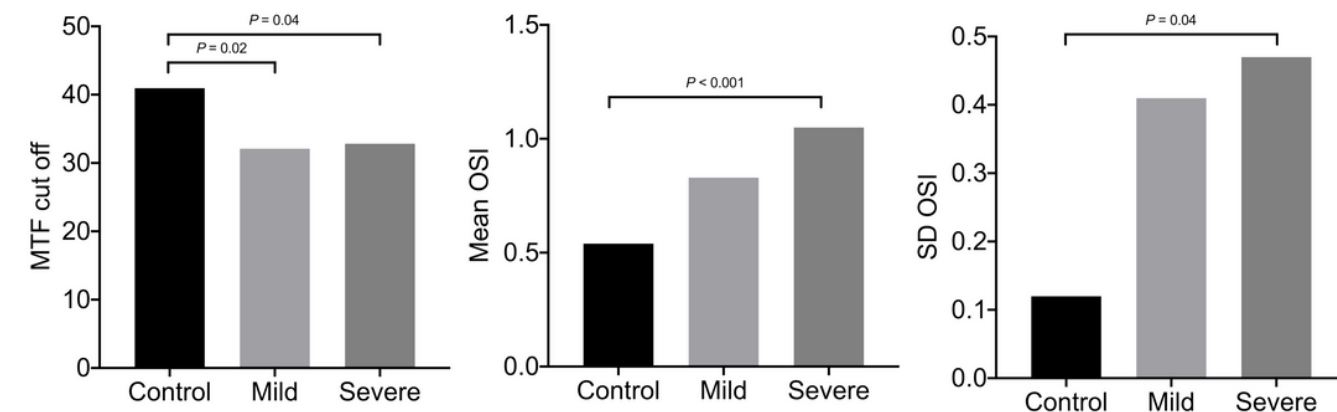


Figure 2

Baseline analysis of optical quality in DED patients and control subjects

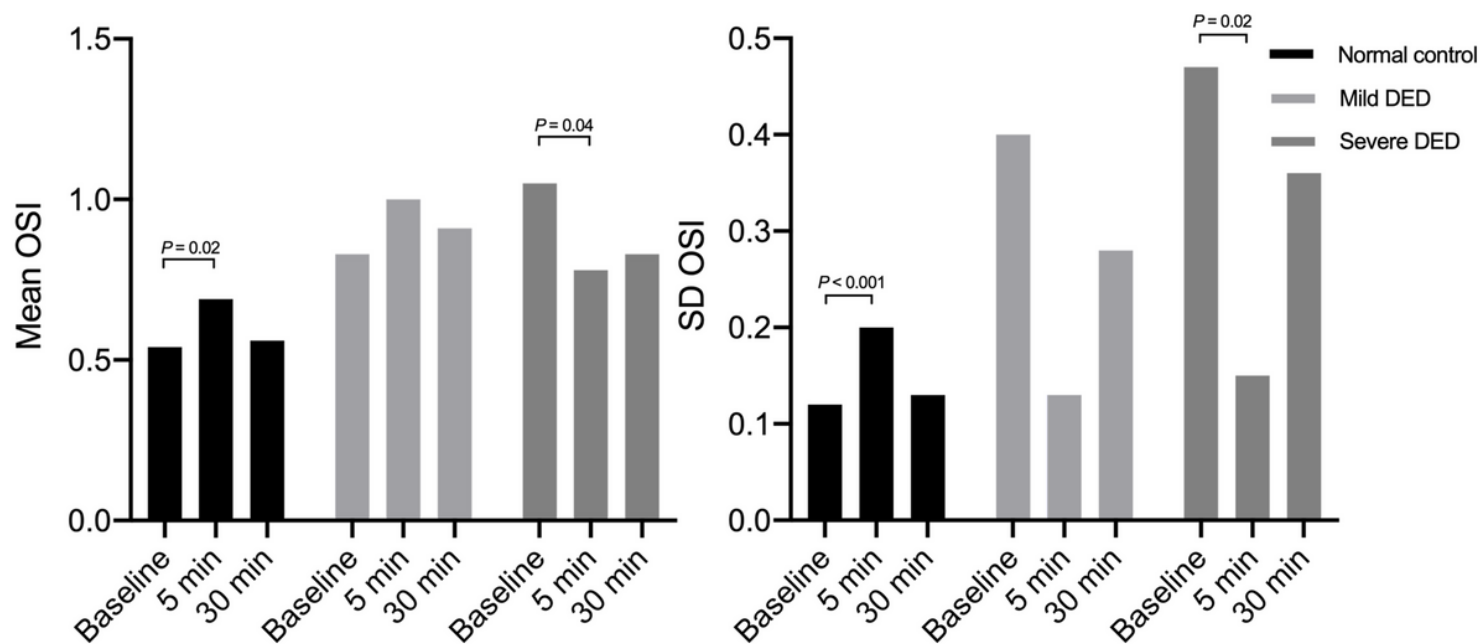


Figure 3

Change in mean OSI and SD OSI from baseline to 5 min and 30 min after AT instillation