

Reliability and Validity of Pelvic Floor Muscle Strength Assessment Using the MizCure Perineometer

Yui Abe-Takahashi

Graduate school of Medicine, Hokkaido University

Takeya Kitta (✉ kitta@fb3.so-net.ne.jp)

Graduate School of Medicine, Hokkaido University

Mifuka Ouchi

Department of Physical Therapy, School of Rehabilitation Sciences, Health Sciences University of Hokkaido

Minori Okayauchi

Department of Rehabilitation, Sapporo Maruyama Orthopedic Hospital

Hiroki Chiba

Department of Renal and Genitourinary Surgery, Graduate School of Medicine, Hokkaido University

Madoka Higuchi

Department of Renal and Genitourinary Surgery, Graduate School of Medicine, Hokkaido University

Mio Togo

Department of Renal and Genitourinary Surgery, Graduate School of Medicine, Hokkaido University

Nobuo Shinohara

Department of Renal and Genitourinary Surgery, Graduate School of Medicine, Hokkaido University

Research article

Keywords: MizCure, Vaginal pressure, Reliability, Validity, Pelvic floor muscles, Perineometer

DOI: <https://doi.org/10.21203/rs.3.rs-45457/v1>

License:  This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Abstract

Background

The purpose of this study was to clarify the reliability and validity of pelvic floor muscle (PFM) strength assessment using the MizCure perineometer in healthy women.

Methods

Twenty healthy women (age 20–45 years) participated in this study. The vaginal pressure measurements using the MizCure and Peritron perineometers were repeated during PFM contraction in the supine and standing positions. All women were evaluated twice by examiners 1 and 2. Following the measurements in the first session (Test 1), they were repeated after an interval of between 2 and 6 weeks (Test 2). Within- and between-session intra- and inter-rater reliabilities in vaginal pressure were analyzed using intraclass correlation coefficients (ICC) (1, 1) and (2, 1), respectively. Validity was assessed by Pearson's product-moment correlation coefficient and Spearman's rank correlation analysis.

Results

Within-session intra-rater reliabilities for both examiners 1 and 2 for all vaginal pressures in Tests 1 and 2 were 0.90 to 0.96 for both perineometers. Between-session intra-rater reliability for the MizCure was 0.72 to 0.79 for both positions for examiner 1, and 0.63 in the supine position and 0.80 in the standing position for examiner 2. Inter-rater reliability for Test 1 was 0.91 in the supine position and 0.87 in the standing position for the MizCure. The vaginal pressures using the MizCure and Peritron were significantly associated with the supine position ($r = 0.68$, $P < .001$) and the standing position ($r_s = 0.82$, $P < .001$).

Conclusion

Measurement of PFM strength using the MizCure perineometer is a reliable and valid method in healthy women.

Background

An important role of the pelvic floor muscles (PFM) is to maintain urine continence and support the pelvic organs. Voluntary PFM contraction is evaluated by assessing pelvic floor elevation, muscle strength, endurance, and coordination [1]. In clinical practice, digital vaginal palpation is the technique most often used to assess PFM function [2].

However, the sensitivity of vaginal palpation for quantifying sustained contractions [3] and discriminating variations in force is less than that of other techniques, and it has been shown to have limited reliability even when performed by experienced examiners [4]. Vaginal pressure measurement is a commonly used quantitative evaluation to measure PFM strength [3], and it is significantly lower in women with stress incontinence than in healthy women [5]. It is also used as a teaching tool and as motivation for conducting training exercises [6]. Thus, vaginal pressure measurement has high clinical importance. It is necessary to perform an objective evaluation of the PFM to be able to properly treat, give feedback, and document changes in PFM function during rehabilitation [7]. Additionally, PFM evaluation is recommended by the International Continence Society and considered essential to assess a post-therapeutic intervention effect [8].

The Peritron (Laborie, Mississauga, ON, Canada) perineometer is commonly available for clinical practice and research. However, in order to import the Peritron into some countries, complicated purchasing procedures are required because this device is considered medical equipment. Therefore, there are some barriers to its use for evaluation and research. The MizCure (OWOMED, Seoul, Korea) is sold as a PFM training and biofeedback device. It can be easily purchased online by private individuals. The MizCure is generally used in some urology and gynecology and urogynecology clinics for training. The MizCure uses different units of measurement, which complicates any comparison of measurements obtained between the MizCure and Peritron perineometers. Whether the measurements obtained using the two perineometers, even with probes of similar diameters, are correlated is not known. In a previous study using the Peritron (Cardio-Design, Oakleigh, VIC Australia), it was found to have good inter-rater reliability, intra-rater reliability, and validity [3, 9–11].

However, the reliability and validity of the MizCure have not been verified. The purpose of this study was to clarify the reliability and validity of PFM strength assessment using the MizCure perineometer in healthy women.

Methods

Subjects

A convenience sample of 20 healthy women was recruited for this study. A sample size calculation showed that 17 subjects were needed for a correlation greater than 0.7, alpha level of 5%, power of 90%, and effect size of 0.6 [12]. In this study, the sample size was set at 20, taking into account 3 dropouts. This study of intra- and inter-rater reliabilities and agreement was performed at our institute from September 2018 to December 2019. The patients included in this study were nulliparous, non-pregnant women, aged 20 to 45 years, with body mass index $<25 \text{ kg/m}^2$ and no gynecological complaints or disease verified, with the ability to correctly contract the PFM. Women with pelvic organ prolapse or who had undergone pelvic reconstructive surgery, those who had symptoms of vaginal infection, intolerance to condoms, or allergy to the gel used in the procedure, as well as those involved in PFM training, were

excluded. The present study was approved by the Scientific Ethics Committee of our institute (#018-0056), and all patients provided their informed consent.

Assessment Tools and Procedures

Assessment tools:

Manometry 1. The Peritron 9300 perineometer (Laborie), shown in Figure 1, was used in this study. The Peritron perineometer has a conical vaginal probe, 26 mm (pressurized: 33 mm) in diameter and 110 mm in length, with a measurable length of 55 mm. The vaginal probe is connected to the perineometer's main body with an 80-cm plastic tube. When the probe is compressed by vaginal pressure, a pressure sensor measures the vaginal pressure. The probe consisted of an air-filled silicone rubber sensor and measured pressure in cmH₂O. The occlusive pressure readings obtained by the perineometer provide surrogate measures of PFM strength.

Manometry 2. The MizCure perineometer (OWOMED, Korea) is a conical vaginal insert, 21 mm (pressurized: 27 mm) in diameter and 79 mm in length, with a measurable length of 50 mm (Figure 2).

The probe was connected to the perineometer's main body via a 75-cm silicone tube. When a silicone tube is connected to the perineometer's main body and the power is turned on, air enters the probe and the probe expands. When pressure is applied to the inside of the vagina to the inflated probe sensor, the pressure sensor measures the vaginal pressure. The inflation pressure can be set to 140 or 150 mmHg. In the present study, the inflation pressure was set to 140 mmHg. The unit measured pressure in mmHg.

Procedure:

Test 1. First, before starting the tests, a transperineal technique using two-dimensional (2D) ultrasound confirmed that each woman was able to contract the PFM correctly based on 2D transperineal ultrasound measurements, including the anteroposterior diameter of the urogenital hiatus (measured at rest and during PFM contraction) (Figure 2). In our group, we demonstrated that 2D transperineal ultrasound is useful to assess PFM function in patients with pelvic organ prolapse [13]. Yang et al. found a close correlation between reduced urogenital hiatus diameter in the sagittal plane and the modified Oxford grading scale [11]. The modified Oxford grading scale is defined as follows: 0 = no contraction; 1 = flicker; 2 = weak; 3 = moderate; 4 = good; and 5 = strong [14]. Second, vaginal pressure was measured with the Peritron and MizCure perineometers. The order of use of the two vaginal manometers and the two test positions were each performed randomly. Testing was conducted with the women in two positions: the supine position, with flexed and slightly abducted legs, and the standing position, with straight and slightly abducted legs. Before data were acquired by the perineometers, the participant inserted the probe, which was covered with a condom and lubricated with hypoallergenic gel, into her vaginal cavity. The participants were instructed to place the probe inside the vagina to a location where 0.5 to 1.0 cm of the probe was visible from the outside of the introitus. PFM strength was then evaluated by a maximum voluntary contraction, as measured by squeeze pressure. The instruction used for each contraction was

'squeeze and lift the PFM as much as you can'. Vaginal pressure testing was performed with three repetitions of maximum voluntary contractions that each lasted for 3 sec, with a 3-sec rest between contractions. A 2-min rest break was then taken. Visible co-contraction of the transversus abdominis muscle was permitted, as long as there was no pelvic tilting [15, 16]. Examiner 1 was a physiotherapist with 11 years of clinical experience. Examiner 2 was a physiotherapist with 5 years of clinical experience and 4 years of educational experience in a university institution.

Test 2. All women were evaluated twice. After the testing protocol was completed in the first session (Test 1), all subjects repeated the protocol 2 to 6 weeks later (Test 2). In Test 2, vaginal pressure measurements were performed using only the MizCure perineometer. The order of the two test positions (supine, standing) and the two examiners were each assigned randomly.

Statistical analysis

Within- and between-session intra-rater reliabilities in vaginal pressure values (maximal voluntary contraction) were analyzed using intraclass correlation coefficients (ICC) (1, 1), and inter-rater reliability was analyzed using ICC (2, 1). Validity was assessed by Pearson's product-moment correlation coefficient and Spearman's rank correlation analysis of the vaginal pressure values of the Peritron and MizCure. Statistical analyses were performed using the free statistical analysis software R, version 2.12.0, with the level of significance set at 5%.

Results

The median age of the 20 healthy female participants was 26.5 years (range 23 to 45 years), and their median body mass index was 19.4 (range 17.5 to 23.4) kg/m². None of the subjects included in the analysis had done PFM training before participating in the research project or between the two evaluation points. Table 1 summarizes within and between-session vaginal pressure values obtained by examiners 1 and 2 (MizCure and Peritron perineometers).

Within-Session Intra-rater Reliability

Table 1 shows the within-session intra-rater reliability using three repetitions of each maximum voluntary contraction by the MizCure and Peritron perineometers for both Tests 1 and 2. For both examiners 1 and 2, all vaginal pressures in Tests 1 and 2 had ICC (1, 1) values of 0.90 to 0.96.

Between-Session Intra-rater Reliability

Between-session intra-rater reliability values for the MizCure perineometer for examiners 1 and 2 are shown in Table 2. The between-session intra-rater reliability of examiner 1 was ICC (1, 1) = 0.72 for the supine position and 0.79 for the standing position. The between-session intra-rater reliability of examiner 2 was ICC (1, 1) = 0.63 for the supine position and 0.80 for the standing position.

Within- and Between-Session Inter-rater Reliabilities

Table 3 shows the inter-rater reliability analysis for vaginal pressure values for Tests 1 and 2. The inter-rater reliability for Test 1 was ICC (2, 1) = 0.96 for both the supine and standing positions for the Peritron. The ICC (2, 1) for MizCure was 0.91 for the supine position and 0.87 for the standing position. The inter-rater reliability of the MizCure in Test 2 was ICC (2, 1) = 0.69 for the supine position and 0.95 for the standing position.

Validity

Significant correlations between the Peritron and MizCure perineometers in the measurements of vaginal pressure were found in the supine position (Pearson's correlation coefficient of 0.68, $P < .001$) and in the standing position (Spearman's correlation coefficient of 0.82, $P < .001$). More details about these results are presented in Table 4.

Discussion

PFM training has been shown to improve stress urinary incontinence and pelvic organ prolapse [17, 18] and is recommended by the International Continence Society as Grade A [19]. However, about 30% of women report failure to contract the PFM correctly [20]. Incorrect PFM contraction is not expected to have a training effect. Therefore, it is recommended that proper PFM training should always include an objective assessment of correct contraction.

In the present study, the reliability and validity of PFM strength assessment using the MizCure perineometer were examined in healthy women. Using transvaginal devices, it is known that the measurement of PFM strength depends on the size and placement of the probe, the subject's cooperation, and the examiner's experience and skills [21, 22]. If a small perineometer probe is used, the placement of the intravaginal probe causes reliability problems, because the probe may be located not completely adjacent to the pressure zone [23]. Thus, in the current study, whether the MizCure can properly measure PFM strength was verified using the widely reported Peritron.

The within-session intra-rater reliability results of the MizCure and Peritron vaginal pressures were ICC (1, 1) 0.90 to 0.96 for both examiners 1 and 2 (Table 1). The intra-rater reliabilities of between-session testing using the MizCure are shown in Table 2. ICC (1, 1) was 0.72 for the supine measurement and 0.79 for the standing measurement for examiner 1 and 0.63 for the supine position measurement and 0.80 for the standing position measurement for examiner 2. In the present study, intra-rater reliability for the MizCure measurement was slightly lower between sessions than within sessions. Furthermore, the results for inter-rater reliability of the two perineometers were as follows: Peritron and MizCure had good inter-rater reliabilities in Test 1 (1st day), with ICC (2, 1) of 0.87 to 0.96 for both supine and standing positions measurements. In Test 2 (2nd day), MizCure measured in the supine position had an ICC (2, 1) = 0.69, slightly lower than in Test 1.

In the previous study on the intra-rater reliability of the Peritron, the ICC (1, 1) was over 0.9 for the supine and standing position measurements [3]. Therefore, the results of the present study suggest that the

within-session intra-rater reliability of the MizCure is as good as that of the Peritron. Rahmani et al. and Ferreira et al. reported the inter-rater reliability of vaginal pressure measurements using the Peritron. Rahmani et al. reported that the between-session ICC (1, 1) was 0.88 [9]. Ferreira et al. reported that the mean vaginal squeeze pressure had good inter-rater reliability, and the difference between the examiners was not significant [10]. In the current study, the between-session intra-rater reliability of the MizCure was slightly lower than that reported by Rahmani et al [9]. This is primarily because of the size and placement of the probes. In the current study, the insertion and placement of the probe were performed by the subject. The MizCure has a smaller probe than the Peritron, and it is difficult to standardize the position of the probe between subjects. The previous study showed that probe placement can affect measurement results [21]. The fact that intravaginal squeeze pressure changes along the vagina [24] means that the profile of vaginal pressure is not fully understood. This suggests that probe placement may have affected reliability. The MizCure probe used in the current study was 79 mm in length. The vaginal high-pressure zone at rest and during PFM contraction is 2 to 4 cm from the vaginal introitus [25]. The vaginal high-pressure zone was shown to be related to the PFM contraction [24]. Therefore, the MizCure probe is considered to cover the high-pressure zone of the vagina. The other factor that may have affected the results for the reliability of vaginal pressure measurements may be the skill of the examiner. With respect to this factor, the two examiners were skilled physical therapists with urologic education. The examiner checked the correct PFM contraction with 2D ultrasound prior to measurement, and always checked to prevent compensatory movement due to PFM contraction (e.g., pelvic tilt or excessive abdominal muscle contractions). Therefore, the effect of the two examiners on the measured value was thought to be small.

ICC reliability criteria are defined as substantial for 0.61 to 0.80 and almost perfect for 0.81 to 1.0 [26]. From this perspective, the present results indicate that the intra-rater reliability of the MizCure within and between days was substantial to almost perfect. The inter-rater reliability was similar. These results suggest that the use of the MizCure perineometer to evaluate PFM strength can minimize the effects of the examiner and provide good intra-rater reliability.

The validity of the MizCure was evaluated using Pearson's product-moment correlation coefficient and Spearman's rank correlation coefficient. The correlation between MizCure and Peritron measurements has not been previously reported. The MizCure measurements showed a significant correlation with the Peritron measurements: $r = 0.68$ for the supine measurements and $r_s = 0.82$ for the standing measurements. For the correlation coefficient, 0.4 to 0.69 is considered moderate and 0.7 to 0.89 strong [27]. Therefore, the correlation coefficients for the MizCure were moderate to high. The results suggest that the MizCure is a suitable tool for measuring PFM strength. There have been reports in the past examining the validity of the Peritron and other perineometers [28]. Barbosa et al. reported the following differences among the other devices: acquisition of higher or lower measurement values depends not only on the diameter of the probes used, but also on other variables, such as individual vaginal diameter, probes of different materials, and differences in the sensitivity of each piece of equipment to vaginal

pressure. Therefore, a detailed examination of the characteristics of the MizCure perineometer and the individual's vagina will be necessary in the future.

The advantage of the MizCure perineometer is that it is easy to purchase, portable, and simple to use. These results suggest that the MizCure is a tool that can quantitatively reflect PFM function, since the reliability and validity of the measured vaginal pressure values are good. This may help select the measurement position for evaluation and treatment purposes and help the treatment plan.

However, as a limitation of this study, the results of the present study are limited to healthy women without PFM dysfunction, such as stress urinary incontinence or pelvic organ prolapse.

Conclusion

The present findings suggest that measurement of PFM strength in the supine and standing positions using the MizCure perineometer is a reliable and valid method for healthy women.

Abbreviations

PFM: pelvic floor muscle; 2D:two-dimensional; ICC:intraclass correlation coefficient

Declarations

Ethics approval and consent to participate

The present study was approved by the Scientific Ethics Committee of Hokkaido University Hospital (#018-0056), and written informed consent was obtained from all the participants.

Consent for publication

Not applicable

Competing interests

The authors declare that they have no competing interests

Funding

none

Authors' contributions

YA: Data collection, management, data analysis, manuscript writing/editing

TK: Protocol/project development, manuscript writing/editing

MO: Data collection, manuscript writing/editing

MOk: Data collection, manuscript writing/editing

HC: Manuscript writing/editing

MH: Manuscript writing/editing

MT: Data collection, manuscript writing/editing

NS: Protocol/project development, manuscript writing/editing

All authors have read and approved the manuscript.

Acknowledgements

Not applicable

Availability of data and materials

The datasets used and/or analyzed during the current study are available from the corresponding author on reasonable request.

References

1. Bø K, Sherburn M. Evaluation of female pelvic-floor muscle function and strength. *Phys Ther.* 2005;85:269–82.
2. Laycock J, Jerwood D. Pelvic Floor Muscle Assessment: The perfect scheme. *Physiotherapy.* 2001;87:631–42.
3. Frawley HC, Galea MP, Phillips BA, Sherburn M, Bø K. Reliability of pelvic floor muscle strength assessment using different test positions and tools. *Neurourol Urodyn.* 2006;25:236–42.
4. Morin M, Dumoulin C, Bourbonnais D, Gravel D, Lemieux MC. Pelvic floor maximal strength using vaginal digital assessment compared to dynamometric measurements. *Neurourol Urodyn.* 2004;23:336–41.
5. Amaro JL, Moreira EC, De Oliveira Orsi Gameiro M, Padovani CR. Pelvic floor muscle evaluation in incontinent patients. *Int Urogynecol J.* 2005;16:352–4.
6. Bø K, Finckenhagen HB. Is there any difference in measurement of pelvic floor muscle strength in supine and standing position? *Acta Obstet Gynecol Scand.* 2003;82:1120–4.
7. Cacciari LP, Kruger J, Goodman J, Budgett D, Dumoulin C. (2020) Reliability and validity of intravaginal pressure measurements with a new intravaginal pressure device: The FemFit®. *Neurourol Urodyn.* 2020;39:253 – 60.

8. Abrams P, Andersson KE, Bircder L, Brubaker L, Cardozo L, Chapple C, et al. Fourth International Consultation on Incontinence Recommendations of the International Scientific Committee: Evaluation and treatment of urinary incontinence, pelvic organ prolapse, and fecal incontinence. *Neurourol Urodyn*. 2010;29:213–40.
9. Rahmani N, Mohseni-Bandpei MA. Application of perineometer in the assessment of pelvic floor muscle strength and endurance: a reliability study. *J Bodyw Mov Ther*. 2011;15:209–14.
10. Ferreira CH, Barbosa PB, de Oliveira Souza F, Antônio FI, Franco MM, Bø K. Inter-rater reliability study of the modified Oxford Grading Scale and the Peritron manometer. *Physiotherapy*. 2011;97:132–8.
11. Yang SH, Huang WC, Yang SY, Yang E, Yang JM. Validation of new ultrasound parameters for quantifying pelvic floor muscle contraction. *Ultrasound Obstet Gynecol*. 2009;33:465–71.
12. Machin D, Campbell M, Fayers P, Pinol A. In sample size tables for clinical studies 2nd edn. In: Axford JS, editor. *The Correlation Coefficient*. USA: Blackwell Science; 1997. p. 168 – 73.
13. Ouchi M, Kitta T, Suzuki S, Shinohara N, Kato K. Evaluating pelvic floor muscle contractility using two-dimensional transperineal ultrasonography in patients with pelvic organ prolapse. *Neurourol Urodyn*. 2019;38:1363–9.
14. Laycock J. Clinical evaluation of the pelvic floor. In: Schussler B, Laycock J, Norton P, Stanton S, editors. *Pelvic Floor Re-education*. London: Springer-Verlag; 1994. pp. 42–8.
15. Sapsford RR, Hodges PW, Richardson CA, Cooper DH, Markwell SJ, Jull GA. Co-activation of the abdominal and pelvic floor muscles during voluntary exercises. *Neurourol Urodyn*. 2001;20:31–42.
16. Neumann P, Gill V. Pelvic floor and abdominal muscle interaction: EMG activity and intra-abdominal pressure. *Int Urogynecol J Pelvic Floor Dysfunct*. 2002;13:125–32.
17. Braekken IH, Majida M, Engh ME, Bø K. Can pelvic floor muscle training reverse pelvic organ prolapse and reduce prolapse symptoms? An assessor-blinded, randomized, controlled trial. *Am J Obstet Gynecol*. 2010;203:170.e1-170.e7.
18. Dumoulin C, Cacciari LP, Hay-Smith EJC. Pelvic floor muscle training versus no treatment, or inactive control treatments, for urinary incontinence in women. *Cochrane Database Syst Rev*. 2018. doi:10.1002/14651858.CD005654.pub4.
19. Dumoulin C, Hunter KF, Moore K, Bradley CS, Burgio KL, Hagen S, et al. Conservative management for female urinary incontinence and pelvic organ prolapse review 2013: Summary of the 5th International Consultation on Incontinence. *Neurourol Urodyn*. 2016;35:15–20.
20. Vermandel A, De Wachter S, Beyltjens T, D'Hondt D, Jacquemyn Y, Wyndaele JJ. Pelvic floor awareness and the positive effect of verbal instructions in 958 women early postdelivery. *Int Urogynecol J*. 2015;26:223–8.
21. Bø K. Pressure measurements during pelvic floor muscle contractions: the effect of different positions of the vaginal measuring device. *Neurourol Urodyn*. 1992;11:107–13.
22. Bø K, Finckenhagen HB. Vaginal palpation of pelvic floor muscle strength: inter-test reproducibility and comparison between palpation and vaginal squeeze pressure. *Acta Obstet Gynecol Scand*. 2001;80:883–7.

23. Dougherty MC, Bishop KR, Mooney RA, Gimotty PA, Landy LB. Variation in intravaginal pressure measurements. *Nurs Res.* 1991;40:282–5.
24. Guaderrama NM, Nager CW, Liu J, Pretorius DH, Mittal RK. The vaginal pressure profile. *Neurourol Urodyn.* 2005;24:243–7.
25. Cacciari LP, Pássaro AC, Amorim AC, Geuder M, Sacco ICN. Novel instrumented probe for measuring 3D pressure distribution along the vaginal canal. *J Biomech.* 2017;58:139–46.
26. Landis JR, Koch GG. The measurement of observer agreement for categorical data. *Biometrics.* 1977;33:159–74.
27. Schober P, Boer C, Schwarte LA. Correlation coefficients: Appropriate use and interpretation. *Anesth Analg.* 2018;126:1763–8.
28. Barbosa PB, Franco MM, Souza Fde O, Antônio FI, Montezuma T, Ferreira CH. Comparison between measurements obtained with three different perineometers. *Clinics.* 2009;64:527–33.

Tables

Table 1

Mean and standard deviation of vaginal pressure values and within-session intra-rater reliability analysis for vaginal pressure values for examiners 1 and 2 (N=20)

| | | | Supine position | | Standing position | |
|------------|--------|-------------------------------|-----------------|---------------------|-------------------|---------------------|
| | | | Mean ± SD | ICC (1, 1) (95% CI) | Mean ± SD | ICC (1, 1) (95% CI) |
| Examiner 1 | Test 1 | Peritron (cmH ₂ O) | 37.5±14.6 | 0.96 (0.93-0.98) | 36.7±10.3 | 0.95 (0.90-0.97) |
| | | MizCure (mmHg) | 25.1±8.1 | 0.92 (0.85-0.96) | 25.0±9.0 | 0.92 (0.84-0.96) |
| | Test 2 | MizCure (mmHg) | 25.1±8.1 | 0.91 (0.82-0.96) | 25.0±9.0 | 0.93 (0.87-0.97) |
| Examiner 2 | Test 1 | Peritron (cmH ₂ O) | 36.4±14.8 | 0.94 (0.89-0.97) | 37.7±10.5 | 0.94 (0.89-0.97) |
| | | MizCure (mmHg) | 26.5±8.3 | 0.90 (0.80-0.95) | 24.6±10.7 | 0.95 (0.91-0.98) |
| | Test 2 | MizCure (mmHg) | 25.5±8.4 | 0.90 (0.82-0.95) | 27.2±10.6 | 0.93 (0.87-0.97) |

Values are presented as mean ± standard deviation (SD).

ICC: intraclass correlation coefficient, CI: confidence interval.

Test 2 was performed 2-6 weeks after Test 1.

Table 2 Between-session intra-rater reliability analysis for the MizCure perineometer for examiners 1 and 2

| ICC (1, 1) (95% CI) | | |
|---------------------|------------------|-------------------|
| | Supine position | Standing position |
| Examiner 1 | 0.72 (0.43-0.88) | 0.79 (0.55-0.91) |
| Examiner 2 | 0.63 (0.28-0.83) | 0.80 (0.57-0.91) |

ICC: intraclass correlation coefficient, CI: confidence interval.

Table 3 Inter-rater reliability analysis for vaginal pressure values for tests 1 and 2

| ICC (2, 1) (95% CI) | | | |
|---------------------|----------|------------------|-------------------|
| | | Supine position | Standing position |
| Test 1 | Peritron | 0.96 (0.91-0.98) | 0.96 (0.89-0.98) |
| | MizCure | 0.91 (0.79-0.96) | 0.87 (0.72-0.95) |
| Test 2 | MizCure | 0.69 (0.38-0.86) | 0.95 (0.89-0.98) |

ICC: intraclass correlation coefficient, CI: confidence interval.

Table 4 Correlation analysis of measurements in the supine position and the standing position

| | Correlation coefficient | p value |
|-------------------|-------------------------|---------|
| | r or r _s | |
| Supine position | 0.68 ^a | < .001 |
| Standing position | 0.82 ^b | < .001 |

^aPearson's product-moment correlation coefficient for MizCure vs Peritron

^bSpearman's rank correlation coefficient for MizCure vs Peritron

Figures

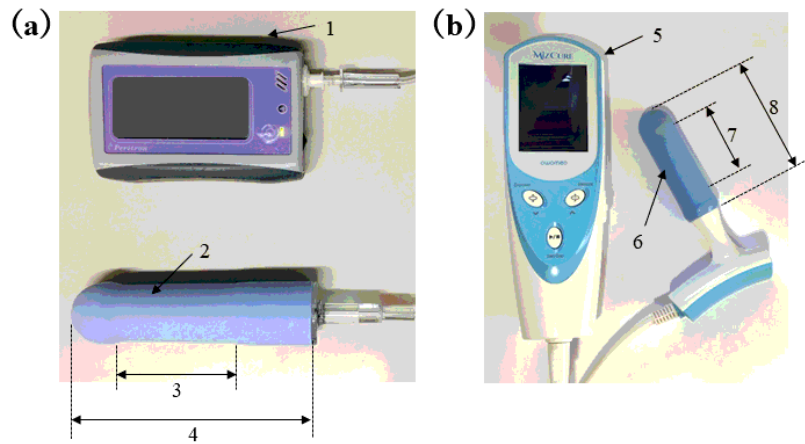


Figure 1

Figure 1

Perineometers used in this study: (a) Peritron 9300 perineometer (Laborie, Mississauga, ON, Canada) with a vaginal probe, 1: Perineometer's main body, 2: Diameter 26-33 (pressurized) mm, 3: Measurable length, 55 mm, 4: Length: 110 mm. (b) MizCure perineometer (OWOMED, Seoul, Korea) with a vaginal probe, 5: Perineometer's main body, 6: Diameter 21-27 (pressurized) mm, 7: Measurable length, 50 mm, 8: Length 79 mm. These pictures were taken our devices in our institute.

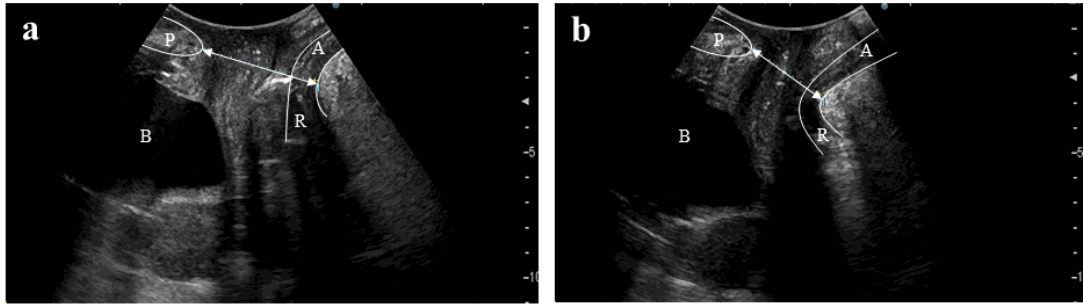


Figure 2

Figure 2

Transperineal mid-sagittal plane ultrasound image in healthy women: At rest (a), during pelvic floor muscle contraction (b). Urogenital hiatus diameter was measured as the distance between the anorectal junction and the inferior border of the pubic symphysis (white double headed arrow). The levator ani muscle was determined based on the hyperechogenic region posterior to the anorectal junction. The correct pelvic floor muscle contraction indicated the cranial ventral displacement of the levator ani muscle, and urogenital hiatus diameter was shortened. A = anus, B = bladder, P = pubic symphysis, R = rectum

Supplementary Files

This is a list of supplementary files associated with this preprint. Click to download.

- [20200812supplementalfile.xls](#)