

Anterior Transpedicle Screw in Lumbosacral Spine and Radiographic Measurements: A Retrospective Analysis

Wei-Xing Xu

Tongde Hospital Of Zhejiang Province

Wei-Guo Ding

Tongde Hospital Of Zhejiang Province

Bin Xu (✉ spotxu@163.com)

Tongde Hospital Of Zhejiang Province <https://orcid.org/0000-0002-8614-953X>

Hong-Feng Sheng

Tongde Hospital Of Zhejiang Province

Di Lu

Tongde Hospital Of Zhejiang Province

Tian-Hong Hu

Tongde Hospital Of Zhejiang Province

Research article

Keywords: anterior transpedicle screw, lumbosacral spine, radiographic measurement, safe operating area

Posted Date: August 10th, 2020

DOI: <https://doi.org/10.21203/rs.3.rs-50034/v1>

License: © ⓘ This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Abstract

Background

The anterior transpedicle screw technique for L5 and S1 is crucial for proper anterior lumbar interbody fusion. This study aimed to determine the projection, screw trajectory angle, and bone screw passageway length (BSPL) of the anterior transpedicle screw in L5 and S1, as well as the screw's insertion regularity and the operating area that is safe for its insertion.

Methods

Forty patients with low back pain, all of whom had lumbar computed tomography scans available, were included in a retrospective analysis. Radiographic parameters were measured, including the distances from the projection to the upper endplate, lower endplate, and midline; the transverse and sagittal screws' angles; and the BSPL. Ten fresh adult cadaveric lumbosacral spine segments were chosen to determine the safe anatomical area at which to operate. Finally, anterior transpedicle screws were inserted in L5 and S1 to determine the regularity of anterior pedicle screw insertion.

Results

We measured the anterior projection parameters, including the distances to the upper endplate (L5: 12.5 ± 1.3 mm; S1: 4.54 ± 0.87 mm), lower endplate (L5: 17.3 ± 1.6 mm), and midline (L5: 6.6 ± 0.7 mm; S1: 6.6 ± 0.6 mm); the screw trajectory angle, including the transverse screw angle (L5: $25.3^\circ \pm 2.8^\circ$; S1: $25.7^\circ \pm 2.6^\circ$), sagittal screw angle (L5: $17.1^\circ \pm 1.7^\circ$; S1: $22.4^\circ \pm 1.1^\circ$); and the BSPL (L5: 48.6 ± 3.5 mm; S1: 48.0 ± 3.5 mm). We then identified the safe operating area and the regularity of L5 and S1 anterior pedicle screw insertions.

Conclusions

We determined the projection, screw trajectory angle, and BSPL of anterior transpedicle screws in L5 and S1, their insertion regularity, and the area in which the operation could be safely performed.

Background

Lumbar interbody fusion is an effective treatment for spinal disease, including recurrent disc degeneration, spondylolisthesis, degenerative disc disease, pseudarthrosis and spine deformity, spine infection, and tumors [1, 2]. Compared with posterior lumbar interbody fusion, anterior lumbar interbody fusion (ALIF) potentially permits more extensive disc removal, avoids scarring of the neural canal, and preserves the posterior elements [3]. Because biomechanical studies and clinical experience suggest that ALIF with posterior pedicle screw (PPS) augmentation (ALIF-PPS) may provide a superior construct, ALIF-

PPS is currently used most often. However, ALIF-PPS would increase the number of incision, the operating time and blood loss. While stand-alone ALIF has potential benefit of shorter operating time, less blood loss and sparing of posterior muscle damage [4, 5].

Hence, numerous studies have designed and applied anterior lumbar internal fixation systems for ALIF. Most of them were vertebral screw-plate fixation systems, whose stability and biomechanical properties were worse than those of the pedicle screw fixation systems [3]. Compared with the vertebral screw-plate fixation system, the pedicle screw fixation system is simple to use and provides good stability for three-column spinal injuries. Thus, augmentation with an anterior pedicle screw (APS) would provide better stability for ALIF. Karim, who presented a technique that allows the ALIF procedure to be augmented with APS (ALIF-APS) fixation, found that the stability of the ALIF-APS technique is comparable to that provided with ALIF-PPS [3]. Karim, however, did not provide the detailed procedure for APS fixation, including the parameters about the projection, screw trajectory angle, and screw depth.

As two of the most frequently involved segments, L5 and S1 have complex anterior anatomy and unique biomechanics, which pose a clinical challenge for anterior surgical treatment. Because of the complex lumbosacral anatomical structure, various complications are associated with ALIF, including vascular complications, bladder, nerve, ureter, and bowel injuries, and abdominal wall problems [6]. With respect to the complex anatomy of the anterior lumbosacral and related surrounding tissue, the concept of a clear space zone (a triangular area on major blood vessels or nerve trunks) in front of the lumbosacral spine emerged [7]. The detailed anatomical parameters of the clear space zone, however, remained unknown.

We therefore conducted this study to obtain radiographic measurements of the anterior transpedicle screw in L5 and S1, which we expected to reveal (1) the position of the anterior pedicle screw projection; (2) the screw's trajectory angle, including the transverse screw and sagittal screw angles; (3) the bone screw passageway length (BSPL); (4) the regularity of anterior pedicle screw insertion; and (5) anatomical parameters of the safe operating area.

Methods

Specimens

Ten dry adult cadaveric lumbosacral spine segments were used in this study. Exclusion criteria for the specimens included (1) presence of destructive pathology (tumor, infection, prior surgery, severe degeneration) and (2) overly osteoporotic bone.

Pedicle guide needle placement

The Ebraheim method [8] was used to determine the pedicle axis and the anterior projection point of L5 and S1. Line X in the transverse plane and line Y in the sagittal plane were drawn on the specimens, as described previously [8]. The two lines intersected on the anterior aspect. This crossing point was determined to be the anterior pedicle axis projection point, which was marked. Guide needles (Kirschner

wire) were inserted from the anterior pedicle axis projection point along lines X and Y, which eventually resulted in 20 needles being inserted to guide the anterior transpedicle screw. C-arm radiography was performed when the front end of the guide needle was at each of four points—anterior projection point, middle of the vertebrae, posterior edge of the vertebrae, the posterior projection point—to ensure accurate positioning of the guide needle.

Parameter measurements

Forty patients with low back pain were retrospectively included, each of whom had undergone lumbar CT scanning. None of the patients had lumbar structural damage, malformations, or a history of surgery. Syngo 3D software (Siemens Medical Solutions USA, Inc., Malvern, PA, USA) was used to perform radiographic measurements (Figure 1), including anatomic parameters of anterior projection (distances to upper endplate, lower endplate, and midline), transverse screw angle, sagittal screw angle, and BSPL. Anatomic parameter measurements were performed using calipers and a standard ruler (precision of 1 mm) for linear measurements. Anatomic parameters included the safe operating area (distance from the abdominal aortic bifurcation to the L5 lower edge, distance from the common iliac vein confluence to the L5 lower edge, horizontal distance from the inner edge of the common iliac vein to the L5 lower edge, distance between S1 holes, L5/S1 vertebral height, and the area in which operating was safe; Figure 2).

Results

Anterior entry point, screw angle, and BSPL of L5 and S1

We measured the anterior projection parameters of L5, including the distance to the upper endplate (12.5 ± 1.3 mm), the lower endplate (17.3 ± 1.6 mm), and the midline (6.6 ± 0.7 mm). We also measured the screw trajectory angle, including the transverse screw angle ($25.3^\circ \pm 2.8^\circ$) and sagittal screw angle ($17.1^\circ \pm 1.7^\circ$), as well as the BSPL (48.6 ± 3.5 mm; Table 1).

Additionally, we determined the anterior projection parameters for S1, including the distance to the upper endplate (4 mm) and the midline (6.6 ± 0.6 mm); the screw trajectory angle, including the transverse screw angle ($25.7^\circ \pm 2.6^\circ$) and sagittal screw angle ($22.4^\circ \pm 1.1^\circ$); and the BSPL (48.0 ± 3.5 mm; Table 1).

Table 1.
Radiographic parameters of anterior entered point, screw angle and
bone screw passageway length in L5 and S1 ($\bar{x} \pm s$, $n = 40$)

	L5	S1
Distance to upper endplate (mm)	12.5 ± 1.3	4.54 ± 0.87
Distance to lower endplate (mm)	17.3 ± 1.6	-
Distance to midline (mm)	6.6 ± 0.7	6.6 ± 0.6
Transverse screw angle (°)	25.3 ± 2.8	25.7 ± 2.6
Sagittal screw angle (°)	17.1 ± 1.7	22.4 ± 1.1
Bone screw passageway length (mm)	48.6 ± 3.5	48.0 ± 3.5

Regularity of anterior pedicle screw insertion

The regularity of L5 anterior pedicle screw insertion is shown in Figure 3 and that of S1 in Figure 4. When the needle is on the anterior projection in the lateral view, it is on the midpoint between the spinous process and the inner edge of the pedicle in the anteroposterior view. When it reaches the posterior vertebral edge in the lateral view, it is on the inner edge of the pedicle in the anteroposterior view. When it reaches the middle of the pedicle in the lateral view, it is on the middle of the pedicle in the anteroposterior view. Finally, when the needle reaches the posterior projection in the lateral view, it is on the outer edge of the pedicle in the anteroposterior view.

Safe operating area

Our study revealed the anatomical parameters of the safe operating area, including the distance from the abdominal aortic bifurcation to the L5 lower edge (40.50 ± 9.40 mm), the distance from the common iliac vein confluence to the L5 lower edge (27.80 ± 8.60 mm), and the horizontal distance from the inner edge of the common iliac vein to the L5 lower edge (37.50 ± 1.30 mm). The study also determined the distance between S1 holes (29.30 ± 1.30 mm), the L5/S1 intervertebral height (17.20 ± 1.50 mm), and the safe operating area (2058.20 ± 84.30 mm²).

Discussion

Since Boucher et al. initially reported use of the posterior transpedicular screw for lumbosacral fusion fixation in 1959 [9], various pedicle screw fixation systems have been used in spinal surgical procedures. They have provided superior postoperative spinal stability and promoted advances in spine surgery [10]. Various studies have researched detailed PPS procedures, including projection parameters, the trajectory angle and depth of the screw [11, 12], and the regularity of pedicle screw insertion [12], each of which is important if PPS is to be performed with high accuracy. Limited studies, however, have reported on the

details of procedures using the APS. As an effective means of pedicle screw fixation, APS not only provides superior postoperative spinal stability for ALIF, but allows a shorter operating time, less blood loss, and minimal posterior muscle damage [4, 5].

We conducted the present study to determine the anatomic and radiographic parameters of L5 and S1, including projection, the screw's trajectory angle, and the depth of the APS. We found limited information in the literature on the location of the anterior projection, which is important for APS performance. Poor placement of the projection may cause the guide needle to be misplaced and result in complications.

The anterior projection in our study was determined based on the method of Ebraheim [8]. The parameters addressed to determine its location included the distance of the APS to the upper endplate, lower endplate, and midline. The screw trajectory angle was also determined based on the method of Ebraheim [8], and the transverse screw and sagittal screw angles were measured. The screw trajectory angles for APS and PPS should be the same in the same patient. Ebraheim [8] reported that the transverse angle of L5 was 40.6 ± 2.6 in men and 39.6 ± 3.2 in women, and the sagittal angle of L5 was 2.7 ± 1.1 in men and 2.6 ± 0.9 in women. To determine the screw trajectory depth, the length of the bone screw passageway was measured. Ebraheim [8] reported that the pedicle length of L5 was 48.3 ± 2.3 mm in men and 48.3 ± 2.4 mm in women. In the present study, anatomic measurements revealed that the bone screw passageway length was 48.6 ± 3.5 mm for L5 and 48.0 ± 3.5 mm for S1.

The BSPL is defined by the length of the screw. Because the vertebra is formed as an irregular cylinder, with the front of vertebral body exhibiting the most anterior border in the lateral view, the needle may perforate the anterolateral cortex, although the lateral view suggests that the needle is still within the vertebra [11]. Therefore, it is important to obtain the ideal needle depth/vertebral width ratio on the lateral view. Weinstein et al. considered the suitable ratio to be 50%–80% [14]. Du et al. suggested that the ratio should be 85%–90% in lumbar vertebrae [15], and Acikbas and Tuncer reported that the suitable ratio was $60\% \pm 9\%$ in lumbar vertebrae [16]. Wang et al. found that the ratio was not the same on different lateral projection angle views even if the real length of the needle in the vertebra remained unchanged [11]. They suggested that the suitable ratio of the needle depth/vertebral width ratio on a standard lateral view varied from $71.53\% \pm 5.72\%$ to $93.28\% \pm 3.72\%$ and that the ratio for L5 was $88.20\% \pm 6.72\%$. More work is obviously needed to establish a suitable ratio for the APS needle depth.

We also evaluated the regularity of APS insertion in this study, which was guided with high accuracy. A previous study [12] reported that the regularity of PPS insertion was apparent when, progressively, the needle reached the posterior projection in the lateral view, was on the outer edge of the pedicle on the anteroposterior view, reached the middle of the pedicle (lateral view), was on the middle of the pedicle (anteroposterior view), reached the posterior vertebral edge (lateral view), and was on the inner edge of the pedicle (anteroposterior view). Wang et al. reported that the posterior projection of PPS was at the 9 o'clock to 11 o'clock position of the left pedicle and at the 1 o'clock to 3 o'clock position of the right pedicle [11]. This regularity also could be applied to the APS when the needle reaches the posterior projection.

Conclusions

We successfully measured the projection, screw trajectory angle, and BSPL of the anterior transpedicle screw in L5 and S1, proved its insertion regularity, and determined the safe operating area. These results can guide APS insertion and improve its accuracy. We plan to use the APS in L5 and S1 based on these results and will evaluate the accuracy of the positioning of the screw.

Abbreviations

ALIF anterior lumbar interbody fusion

APS anterior pedicle screw

BSPL bone screw passageway length

PLIF posterior lumbar interbody fusion

PPS posterior pedicle screw

Declarations

Ethics approval and consent to participate

This study was approved by the Ethics Committee of Tongde Hospital of Zhejiang Province, and the methods were carried out in accordance with the approved guidelines.

Consent for publication

Not applicable

Availability of data and materials

The datasets used and/or analysed during the current study are available from the corresponding author on reasonable request.

Competing interests

The authors declare that they have no conflicts of interest.

Funding

The study was supported by the Zhejiang Province Public Welfare Technology Application Research Project (CN) (LGF19H060006).

Authors' contributions

XW: project development, manuscript writing, funding acquisition. XB: data collection, data analysis, manuscript writing. DW: data analysis, manuscript writing. SH: project development, data collection. LD: data analysis, supervision. HT: data collection, supervision

Acknowledgment

We thank Nancy Schatken BS, MT(ASCP), from Liwen Bianji, Edanz Group China (www.liwenbianji.cn/ac), for editing the English text of a draft of this manuscript.

References

1. Giang G, Mobbs R, Phan S, et al. Evaluating outcomes of stand-alone anterior lumbar interbody fusion: a systematic review. *World Neurosurgery*. 2017; 104: 259-271.
2. Hoff E K, Strube P, Pumberger M, et al. ALIF and total disc replacement versus 2-level circumferential fusion with TLIF: a prospective, randomized, clinical and radiological trial. *European Spine Journal*. 2015; 24(10):1-3.
3. Karim A, Mukherjee D, Ankem M, et al. Augmentation of anterior lumbar interbody fusion with anterior pedicle screw fixation: demonstration of novel constructs and evaluation of biomechanical stability in cadaveric specimens. *Neurosurgery*. 2006; 58(3):522-527.
4. Choi KC, Kim JS, Shim HK, et al. Changes in the Adjacent Segment 10 Years After Anterior Lumbar Interbody Fusion for Low-Grade Isthmic Spondylolisthesis. *Clinical Orthopaedics & Related Research*. 2014; 472(6):1845.
5. Wang WJ, Chen WK, Yan YG, et al. Application of anterior debridement and reconstruction with anatomical screw-plate fixation for lumbosacral tuberculosis: A 2-year-plus follow-up. *Medicine*. 2017; 96(26):e7103.
6. Wang W, Liu S, He G, et al. Application of Laparoscopic Lumbar Discectomy and Artificial Disc Replacement: At Least Two Years of Follow-Up. *Spine*. 2016; 41 Suppl 19(19):B38.
7. Inamasu J, Kim DH, Logan L. Three-dimensional computed tomographic anatomy of the abdominal great vessels pertinent to L4-L5 anterior lumbar interbody fusion. *Minim Invasive Neurosurg*. 2005; 48(03):127-131.
8. Ebraheim NA, Jr RJ, Xu R, et al. Projection of the lumbar pedicle and its morphometric analysis. *Spine*. 1995; 21(3):233.
9. Boucher HH. A method of spinal fusion. *Journal of Bone & Joint Surgery-british Volume*. 1959; 41(2):248-259.
10. Kasten MD, Rao LA, Priest B. Long-term results of iliac wing fixation below extensive fusions in ambulatory adult patients with spinal disorders. *Journal of Spinal Disorders & Techniques*. 2010; 23(7):37-42.
11. Wang G, Yang H, Chen X, et al. Standard fluoroscopic views in cadavers for determining the entry point and depth of a guide needle for use in transpedicular procedures of the thoracolumbar spine.

Journal of Clinical Neuroscience. 2010; 17(5):588-591.

12. Bai JY, Zhang W, An JL, et al. True anteroposterior view pedicle screw insertion technique. Therapeutics & Clinical Risk Management. 2016; 12(Issue 1):1039-1047.
13. Choi KC, Kim JS, Shim HK, et al. Changes in the Adjacent Segment 10 Years After Anterior Lumbar Interbody Fusion for Low-Grade Isthmic Spondylolisthesis. Clinical Orthopaedics & Related Research. 2014; 472(6):1845.
14. Weinstein JN, Spratt KF, Spengler D, et al. Spinal pedicle fixation: reliability and validity of roentgenogram-based assessment and surgical factors on successful screw placement. Spine. 1998; 13(9):1012.
15. Xin DU, Zhao LX, Qi bin YE. Radiological anatomy study in selecting the length of pedicle screw in lumbar spine. Chinese Journal of Clinical Anatomy. 2002; 20:15–7. [in Chinese]
16. Acikbas SC, Tuncer MR. New method for intraoperative determination of proper screw insertion or screw malposition. J Neurosurg. 2000; 93(1 Suppl): 40-4.

Figures

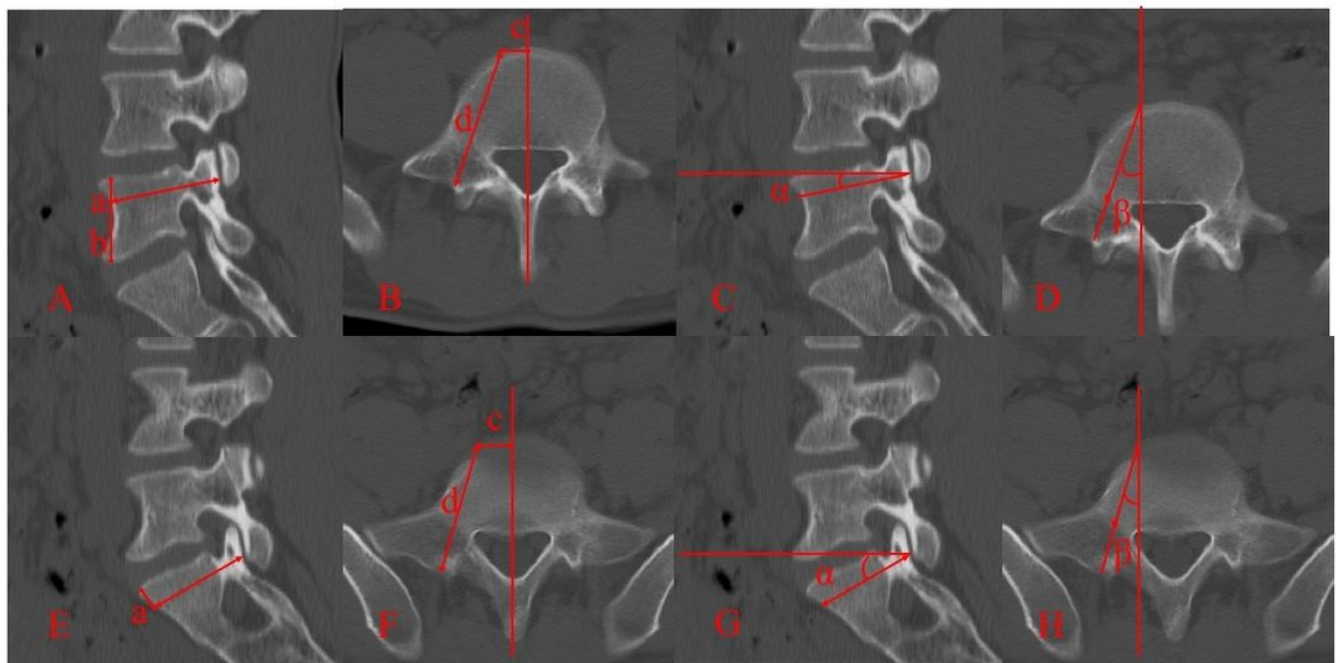


Figure 1

Radiographic parameter measurements were performed, including: anatomic parameters of anterior projection (the distances to upper endplate, lower endplate and midline), transverse screw angle, sagittal screw angle and BSPL.



Figure 2

The safe operating area



Figure 3

The regularity of L5 anterior pedicle screw insertion

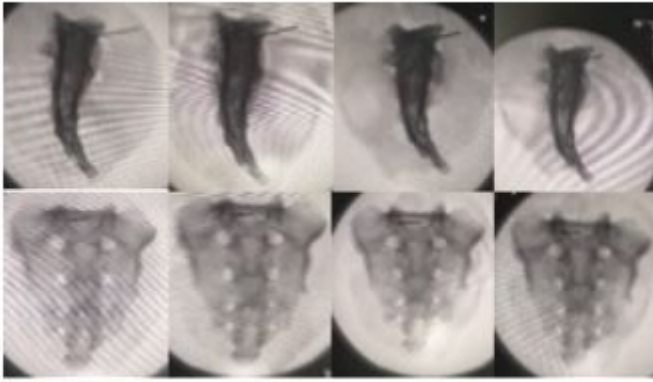


Figure 4

The regularity of S1 anterior pedicle screw insertion