

Effects of Task-Specific Virtual Reality Training Using a Leap Motion Controller on Hemiparetic Upper Extremity in Patients with Stroke

Kenneth N. K. Fong (✉ rsnkfong@polyu.edu.hk)

Department of Rehabilitation Sciences, The Hong Kong Polytechnic University <https://orcid.org/0000-0001-5909-4847>

Y. M. TANG

Hong Kong Polytechnic University Faculty of Engineering

Karen SIE

Hong Kong Polytechnic University Faculty of Health and Social Sciences

Andy K. H. YU

Hong Kong Polytechnic University Faculty of Health and Social Sciences

Cherry C. W. LO

Hong Kong Polytechnic University Faculty of Health and Social Sciences

Yuko W. T. MA

Hong Kong Polytechnic University Faculty of Health and Social Sciences

Research

Keywords: stroke, upper extremity, task-specific training, virtual reality, Leap Motion Controller

Posted Date: August 18th, 2020

DOI: <https://doi.org/10.21203/rs.3.rs-55924/v1>

License: © ⓘ This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Abstract

Background: Task-specific training has been proven to be effective in promoting recovery of the hemiparetic upper extremities after a stroke. This study was to develop a new and innovative task-specific VR (TS-VR) program using a Leap Motion Controller VR device and the Unity3D program for distal hand function training, and to investigate whether a two-week program of TS-VR training would promote recovery of the hemiparetic upper extremity in patients with chronic stroke.

Methods: We designed the TS-VR program based on seven general hand function tasks used in the activities of daily living that require upper limb movement, such as pushing open a door and pouring water. Then, we examined the content validity of the TS-VR according to the views of an expert panel and through field testing on patients with stroke. The final version of the TS-VR was tested on 20 patients suffering from chronic stroke with upper extremity hemiparesis over 2 weeks, 5 sessions per week, 30 minutes per session. Outcomes were assessed using the Fugl-Meyer Assessment-Upper Extremity score (FMA-UE), the Wolf Motor Function Test (WMFT), and the Motor Activity Log (MAL). Data were collected at the first session (week 0), last session (week 2), and follow-up session (week 5). Patients' arm impairments were stratified into lower- and higher-functioning groups according to the Functional Test for the Hemiplegic Upper Extremity (FTHUE).

Results: Significant improvements in upper extremity functions were found after TS-VR training in FMA-UE Total score ($\chi^2=34.219$, $p=0.000$), FMA-UL subscore ($\chi^2=31.2$, $p=0.000$), FMA-Hand subscore ($\chi^2=22.6$, $p=0.000$), and WFMT score ($\chi^2=27.8$, $p=0.000$) among the three time occasions, but no significant effect on grip strength was found. Moreover, the higher-functioning group (levels 5-7 in FTHUE) benefited more from the TS-VR, as indicated in outcome measures of FMA-UL, FMA-Hand, FMA-UE Total, and WMFT respectively, as well as amount of use score in MAL, but this was not the case for those in the lower-functioning group (levels 1-4 in FTHUE).

Conclusions: Our findings suggest that our new TS-VR training system was useful for upper extremity recovery in patients with chronic stroke. It has potential to be applied in clinical settings in future.

Introduction

Upper extremity hemiparesis is one of the major concerns for patients who have suffered a stroke following their discharge from hospital. Over 60% of chronic stroke patients have motor dysfunction in their upper extremities, with only 5% demonstrating complete functional recovery [1]. Among them, only 5–20% of acute stroke patients regained full function, while 33–60% continued to have limited function after 6 months [2].

According to the current international clinical guidelines for stroke management, intensive and frequent practice of task-specific training in the activities of daily living (ADL) has been proven to be effective in promoting recovery of the upper extremities following a stroke [3]. Many research findings have indicated that the best way to relearn a given functional task in ADL is to train specifically for that task through

repetitive and consistent practice [4]. Task-specific training has the benefits of promoting cortical reorganization and associated functional improvements, hence, the rehabilitation outcomes are more successful when the tasks are meaningful to the person [5]. Previous studies have found that task-specific upper limb training can lead to significant improvements in motor function and daily use of the hemiparetic limb among stroke patients [6, 7]. There is also an increasing trend for task-specific training to move away from traditional approaches that uses objects in ADL towards the use of novel technology so as to meet the evolving needs of stroke patient care [8].

Virtual reality is nowadays widely used as part of rehabilitation because of its ability to bridge the gap between laboratory training and the real-life tasks involved in daily living. Virtual reality (VR) is a technology that allows people to view, navigate, and interact with a simulated three-dimensional world in real time. VR comes with different kinds of interactivity according to different immersion levels. Two of its advantages are that it poses no threat to or physical limitations upon patients in the simulated environment, and it can easily be modified to change levels of difficulty, which may not be possible in the real world [9]. It also has advantages over normal computer-based rehabilitation programs. It can address real-time aspects of information processing, enhance dynamic interaction with the virtual environment, and promote patients' intention and willingness to do training [10]. Moreover, a VR environment allows real-time data to be collected and analyzed, so that therapists can adjust and monitor patients' progress in order to increase the efficiency and effectiveness of rehabilitation [11]. There is mounting evidence showing that VR technology provides therapeutic benefits in the improving of the motor function of the upper extremities during stroke rehabilitation [12]. However, most existing VR-based rehabilitations focus on training of the proximal upper extremity, and there is limited research on its effectiveness on the distal upper extremity [13]. For this reason, it would be useful to develop a task-specific VR training program for a hemiplegic hand and examine its effectiveness on patients following a stroke.

The VR system comprises five classical elements. These are the VR engine; input and output devices; the software and database; the user; and the task. Unity3D is a cross platform game engine used to develop 3D games and applications for computer, consoles, websites, and mobile devices. The input and output devices include traditional Head-Mounted Display (HMD), VR gloves, etc. Recently, HoloLens was developed, providing holographic experiences for the user and allowing interaction with digital content dynamically in real time [14]. These devices, however, are usually expensive and complicated. On the other hand, a lot of VR training focuses on collecting patients' cognitive performance data rather than their physical performance and motion data. The Leap Motion Controller (LMC), shown in Fig. 1, is a modern, low-cost, contact-free, and portable input device used for real-time gesture and position tracking of hands [15]. The accuracy of fingertip position tracking is very precise (approximately 0.01 millimeter) [16, 17]. Given these benefits, it was judged that the LMC could best serve as a cost-effective input device for motor recovery training focused on the distal upper extremity.

Recently, Fernández-González et al. [18] designed a video game-based therapy that used the LMC to provide upper limb rehabilitation for patients with Parkinson's disease. The LMC was used to capture the movement of the patient's forearms and hands. Wang et al. [19] explored the effects of a Leap Motion-

based virtual reality system on subacute stroke. The trainings were designed based on the pinching, grasping, and individuating motor skills of fingers. Home-based training is particularly important for patients after hospital discharge, allowing them to practice within a familiar environment, as well as better enabling them to recall their memories during daily practices. In this study, we sought to substantiate an innovative treatment that involves promoting the use of the hemiparetic upper extremity in chronic stroke patients by developing a VR task-specific training program with three stages. In stage 1, we aimed to design a new and innovative task-specific VR program (TS-VR) using Unity3D and LMC as input devices. The program consists of seven general hand function tasks involved in ADL. In stage 2, we examined the content validity of the TS-VR according to the views of an expert panel and through field testing on patients with stroke. In stage 3, we aimed to recruit patients with stroke to participate in our two-week TS-VR training program. Our purpose was to investigate its clinical utility. In particular, we wanted to determine whether the lower functioning or the higher functioning group of clients with paretic upper extremity functional impairment would benefit more from the TS-VR program. The findings of this study could further contribute to the effective care of those with stroke by helping to extend the application of TS-VR to home-based training, as well as to rehabilitation in hospitals and community settings.

Methods

Participants

Twenty patients with stroke were recruited from within a community self-help group for stroke, using convenience sampling. The inclusion criteria were: (1) stroke with unilateral hemispherical involvement; (2) aged 18 or above; (3) stroke onset of six months or more before the study; (4) able to understand verbal instructions and follow one-step commands; (5) no excessive spasticity, defined as a score of 2 or higher on the Modified Ashworth Scale [20]; (6) no complaints of excessive pain or swelling over the paretic upper extremity; (7) no prior participation in any experimental or drug studies within one month; and (8) able to understand the meaning of the study and give informed consent to participate. The choice of a post-stroke period of six months or above as an inclusion criterion for patients with chronic stroke reflected the probability that any spontaneous recovery would have slowed down by the time of the study, thus enabling more brain reorganization in response to the therapeutic intervention under study. Before commencement of the study, written and informed consent was obtained from all patients. The study was carried out in accordance with the principles of the Declaration of Helsinki. Ethical approval was sought and obtained from the Human Ethics Committee of the Hong Kong Polytechnic University (Ref. no.: HSEARS20180503002).

In order to investigate which level of severity of upper extremity impairment would benefit more from the treatment, patients were further stratified into two groups according to whether their hemiparetic upper extremity functional impairment was severe to moderate or mild: Group 1, the lower functioning group, included eight patients with severe to moderate impairments to a hemiparetic upper extremity (i.e., FTHUE level 1–4) who were able to move with bilateral arms, to demonstrate a mass flexion pattern in the

shoulder/elbow, then an active extension control of the shoulder/elbow; Group 2, the higher functioning group, included 12 patients with moderate to mild hemiparetic upper extremity impairments (i.e., FTHUE level ≥ 5) who were able to demonstrate the beginnings of an ability to combine components of strong mass flexion and strong mass extension patterns, and who were able to perform some release of the hand, as well as isolated control of forearm and hand with fair strength.

Task-specific virtual reality training program (TS-VR)

In stage 1, we developed the TS-VR using Unity3D (version 2017.3.1f1) and the LMC (version 3.2.1) as input devices for capturing real-time 3D positioning of the hand. The computer programming language C# was used in the development of the training programming. The TS-VR consists of seven general hand function tasks involved in ADL. These are designed according to the severity of the specific upper limb impairment of stroke patients, with reference to the levels 1–7 in the Functional Test for the Hemiplegic Upper Extremity (FTHUE) [21, 22]. The standardized tasks in the program for each level of impairment were carried out by the performing of discrete movements used in functional activities. These included bilateral and unilateral use of both hands, range of motion tasks, pronation and supination, and grasp and release (e.g., pouring water from a bottle) with the affected upper limb. The training tasks used in the TS-VR program and the corresponding levels (1–7) in the FTHUE are: Level 1 - Pushing a door with both hands (non-affected hand holding affected forearm); Level 2 - Picking up a cup from affected side of the table and moving to non-affected side; Level 3 - Holding a pouch in a static position for 15 seconds; Level 4 - Picking up a cup from non-affected side of the table and moving to affected side; Level 5 - Picking up a water bottle and pouring water into a cup; Level 6 - Picking up a book and placing it on a bookshelf; and Level 7 - Pressing the password pad. Figure 2 shows a screenshot of selected training tasks used in the training program, such as pushing open a door, pouring water, and pressing a button.

Unity3D is a cross-platform game engine that has been widely adopted by various industries for the development of VR programs, augmented reality (AR) games, computer simulations, and other experiences. Figure 3 shows the workflow of the development process for the TS-VR program. The 3D virtual environment and models are first created using SolidWorks. The models are then exported to FBX format and imported to the gaming engine. The imported models are usually gray in color, and the Unity engine supports and provides a physically based rendering material system to create realistic textures and color in various virtual scenes. Custom textures like wood and bricks can be added to the 3D models. The engine also provides a user-friendly interface for the adjusting of material values and parameters, such as “Metallic” and “Smoothness”. This enables the creation of a natural virtual environment under different lighting in real time.

The LMC is used to capture the 3D position of the hand, including the wrist and fingers. The LMC has a one-meter hemispherical view area with a 150 degrees field of view, and it can track users’ finger movements at a rate of over 300 frames per second, such that the screen display changes continually along with the user’s every movement. The LMC uses structured infrared light emitters to create a 3D depth map with two cameras. The cameras capture data in the form of grayscale stereo images and process this data by extracting tracking information such as the position of wrist and fingers. The

tracking algorithms then interpret the 3D data and infer the positions of the hand [23]. Using the LMC, the feature points in the wrist and fingers are extracted to interpolate the motion of the hand.

The LMC works using the Cartesian coordinate system in millimeters (mm). At the beginning, the origin is located at the middle of the device. These coordinates are converted to screen coordinates depending on the screen size or window size of the application, calculated by Eq. 1 [24]:

$$(V_x, V_y) = \left(\frac{(O_x \times U_x \times 2)}{U_x} + \frac{U_x}{2}, U_y - O_y \right) \quad (1)$$

,where V_x and V_y are the x - and y -coordinates with respect to (w.r.t.) the screen coordinates; U_x and U_y are the width and height of the window; and O_x and O_y are the x - and y -coordinates w.r.t. the LMC coordinates.

To train the Hemiplegic Upper Extremity functions of the patients, interactions between different virtual models in the TS-VR training program are required. For instance, when patients push a door or press the password pad, the door will open and the password will display on the screen. In this case, a collider defined by common primitives in the space of the virtual objects is used to determine the interaction with the patients. A collider is a bounding box (Fig. 3) surrounding the virtual models. An interaction is triggered when the distance between the models and the finger is smaller than the distance threshold. Figure 1b shows the pseudo code of the pressing password pad task. In this task, the password is randomly generated. When the virtual hand model triggers the collider, the corresponding password number will be recorded and compared with the generated password. The task ends when the password is correct; otherwise, this task will restart. Similarly, other tasks, such as holding a handbag or placing an object also need to trigger the collider, and then a check is done to determine whether the task has been completed.

Rehabilitation and assessment

In stage 2, we sought qualitative comments for the TS-VR from an expert panel, composed of 10 occupational therapists, each with at least three years of experience in stroke rehabilitation. The panel interviewed 10 clients with stroke of various impairment levels recruited by convenience sampling in the community. After the interview, object component, program structure, and demonstration videos of the program were modified according to the comments of the panel, but the VR tasks remained similar in terms of content and difficulty.

In stage 3, we investigated whether a two-week program using TS-VR training would promote recovery of the paretic hand in patients with chronic stroke, using a single group longitudinal design study. Twenty patients were invited to participate in the TS-VR at the university laboratory. There were a total of 10 sessions, each 30 minutes in length, held five days per week over two consecutive weeks.

The equipment was set up as shown in Fig. 1. The LMC was installed on the table located in front of the monitor. The patients were seated in front of the computer and provided with enough space for them to move the upper extremity in order to complete the TS-VR tasks. The tasks were displayed on the computer monitor in front of the patients. The study was carried out under the one-to-one supervision of an occupational therapy student who was one of the investigators and had undergone training in using the TS-VR. Patients were instructed to sit on the chair, or else on their own wheelchair. The LMC was placed on another chair, in front of the participant and at an appropriate distance to ensure best sensitivity. In the first session, demonstrations were given by the investigator for each level of the TS-VR training tasks to ensure that patients understood how to perform the task correctly. In the following training sessions, the training regimens were tailored to the needs of the patients by adjusting the modes of training (i.e., the progressive and repetitive mode, respectively). For progressive mode, patients were instructed to perform the TS-VR tasks from level 1 to the highest level they could attain. For repetitive mode, patients were instructed to perform a specific task level repetitively for 5–10 minutes. Both progressive mode and repetitive mode were used in each 30 minutes training session, depending on patients' needs, performance, and fatigue level. Patients with lower functioning (FTHUE of 1–4) were allowed to perform the TS-VR training task level 1 or 2 with the assistance of the non-affected hand.

At the beginning, during, and after each training session, patients were allowed to take a rest and do stretching exercises to relieve any tightness, tiredness, or discomfort of their paretic upper extremity. During the training, verbal and tactile cues were given by the investigator to correct patients' abnormal posture and associated movement when they were performing the TS-VR tasks. Visual and audio cues which were built-in to the TS-VR also provided sensory feedbacks to the patients. The time and error records after each completion were also recorded in order to provide immediate feedbacks to the patients.

Outcome measurements

Outcome measurements were conducted at baseline (pre-treatment, first session, week 0), post-treatment (last session, week 2), and follow-up (week 5) at the university laboratory. The primary outcomes were two laboratory-based assessments for arm functions, including the Fugl-Meyer Assessment-Upper Extremity score (FMA-UE) [25, 26] and the Wolf Motor Function Test (WMFT) [27]. The FMA-UE [28] is a well-known impairment test which evaluates patients with stroke through selective movements. The upper limb subscore consists of 32 items, each of which represents movement components, scored on a three-point scale (0, 1, 2). A higher score denotes a better recovery. The WMFT was chosen because the score range of this test is relatively greater and therefore more suitable for capturing both higher and lower levels of arm functioning in stroke patients [29]. The secondary outcome was a self-reported questionnaire, the Motor Activity Log (MAL) (including the Amount of Use scale (AOU) and the Quality of Movement scale (QOM)), indicating how often and how well patients used their affected arm in ADL [30]. It was administered for the actual arm use of the affected hand in daily life. It was carried out by asking patients about the use of their hemiparetic upper limb in 30 daily living activities over one week. Both subscales in the MAL - the AOU and the QOM - were shown to the patients while going through each item over the course of a semi-structured interview.

Statistical analysis

Data analysis was performed using SPSS. Baselines, including demographic data and pre-treatment scores for the outcome measures, were calculated according to descriptive statistics. Nonparametric tests were used because the data collected was either categorical or because sample size was small. The Friedman Test was used to evaluate any significant difference in the hand functions and arm use of patients before and immediately after the training and at within-group follow-up sessions. The Wilcoxon Signed-Rank Test was used for post hoc analysis, in which the measurements taken for each variable on the three occasions (i.e., before and immediately after the training, and at follow-up) were compared to determine where any significant differences lay. The level of significance was set at $p \leq 0.05$ for the Friedman Test after Bonferroni adjustment ($0.05/n$; n = number of tests). The Friedman Test and the Wilcoxon Signed-Rank Test were later used for separate analyses when the patients were stratified into lower-functioning and higher-functioning groups according to the severity of their hemiparetic arm functional impairment.

Results

Patients' demographic characteristics are listed in Table 1. Tables 2 shows the results of primary and secondary outcome measures at the baseline, post-test, and three-week follow-up evaluations for the whole sample and the higher or lower function groups.

Table 1
Baseline Demographics of Study Participants

Characteristics	All (n = 20)	Group 1 Higher Functioning (n = 12)	Group 2 Lower Functioning (n = 8)
Gender, n(%)			
Male	15(75.0)	10(83.3)	5(62.5)
Female	5(25.0)	2(16.7)	3(37.5)
Age, \pmSD	62.0 \pm 5.1	60.9 \pm 5.1	63.6 \pm 5.0
Onset to treatment (months), mean \pm SD	37.4 \pm 31.1	33.3 \pm 33.2	43.6 \pm 28.7
Education, n(%)			
Primary	2(10.0)	2(16.7)	0(0)
Lower secondary	13(65.0)	8(66.6)	5(62.5)
Higher secondary	5(25.0)	2(16.7)	3(37.5)
Tertiary	0(0)	0(0)	0(0)
Type of Stroke, n(%)			
Ischemia	14(70.0)	11(91.7)	3(37.5)
Hemorrhage	6(30.0)	1(8.3)	5(62.5)
Right Hand Dominance, n(%)	20(100.0)	12(100)	8(100)
Hemiparetic Side, n(%)			
Left	9(45.0)	4(33.3)	5(62.5)
Right	11(55.0)	8(66.7)	3(37.5)
Levels of FTHUE, n(%)			
1	1(5.0)	0(0)	1(12.5)
2	2(10.0)	0(0)	2(25.0)
3	1(5.0)	0(0)	1(12.5)
4	4(20.0)	0(0)	4(50.0)
5	0(0)	0(0)	0(0)
6	4(20.0)	4(33.3)	0(0)
7	8(40.0)	8(66.7)	0(0)

Note: FTHUE = Functional Test for the Hemiplegic Upper Extremity

Table 2

Differences in Primary and Secondary Outcome Measures at Pretest, Posttest, and Follow-up in the sample of 20 patients

Outcome measures	Groups	Pretest (1)	Posttest (2)	Follow-up (3)	χ^2	p	Multiple Comparisons	
FMA-UL	All	23.7 ± 7.2	28.1 ± 8.1	28.4 ± 8.3	31.20	0.000**	1, 2	1, 3
	Group 1	26.6 ± 5.2	32.2 ± 4.2	33.1 ± 3.7	21.33	0.000**	1, 2	1, 3
	Group 2	19.4 ± 7.9	22.0 ± 8.9	21.3 ± 8.4	10.57	0.005**	1, 2	1, 3
FMA-Hand	All	17.1 ± 8.2	20.0 ± 8.4	20.7 ± 8.5	22.58	0.000**	1, 2	1, 3
	Group 1	22.1 ± 3.3	24.7 ± 3.2	25.6 ± 2.4	15.80	0.000**	1, 2	1, 3
	Group 2	9.5 ± 7.5	13.0 ± 9.1	13.4 ± 9.3	6.91	0.032*	1, 2	1, 3
FMA-UE Total	All	41.2 ± 14.5	48.2 ± 15.9	48.8 ± 16.2	34.22	0.000**	1, 2	1, 3
	Group 1	49.4 ± 6.6	57.0 ± 6.7	58.2 ± 5.9	21.38	0.000**	1, 2	1, 3
	Group 2	28.9 ± 14.5	35.0 ± 17.0	34.6 ± 16.8	13.71	0.001**	1, 2	1, 3
WMFT	All	44.1 ± 17.9	52.4 ± 19.2	53.1 ± 20.7	27.80	0.000**	1, 2	1, 3
	Group 1	54.3 ± 9.5	64.0 ± 7.1	65.4 ± 8.8	16.87	0.000**	1, 2	1, 3
	Group 2	28.8 ± 16.7	35.1 ± 18.7	34.5 ± 19.7	13.00	0.002**	1, 2	1, 3
Grip strength	All	13.0 ± 7.8	14.2 ± 8.4	14.1 ± 9.3	0.97	0.615		
	Group 1	16.5 ± 6.7	18.0 ± 7.3	19.2 ± 1.9	4.17	0.124		
	Group 2	7.7 ± 6.6	8.5 ± 6.7	6.4 ± 4.9	5.85	0.054		

Note: *p < 0.05; **p < 0.01; Group 1 = Higher functioning group; Group 2 = Lower functioning group; FMA-UE Total score = Fugl-Meyer Assessment-Upper Extremity total score; FMA-Hand = Fugl-Meyer Assessment Upper Limb subscore; FMA-Hand = Fugl-Meyer Assessment Hand subscore; WMFT = Wolf Motor Function Test; MAL-AOU = Motor Activity Log - Amount of Use scale (AOU); MAL-QOM = Motor Activity Log - Quality of Movement scale (QOM)

Outcome measures	Groups	Pretest (1)	Posttest (2)	Follow-up (3)	χ^2	p	Multiple Comparisons		
MAL-AOU	All	2.0 ± 1.5	2.6 ± 1.7	2.8 ± 1.7	24.62	0.000**	1, 2	1, 3	
	Group 1	2.8 ± 1.3	2.6 ± 1.1	3.6 ± 1.2	16.67	0.000**	1, 2	1, 3	2, 3
	Group 2	0.7 ± 0.6	0.6 ± 0.6	1.1 ± 1.0	12.33	0.002**		1, 3	2, 3
MAL-QOM	All	1.8 ± 1.4	2.3 ± 1.4	2.5 ± 1.5	26.64	0.000**	1, 2	1, 3	
	Group 1	3.2 ± 1.0	3.9 ± 0.9	3.5 ± 0.6	13.61	0.001**	1, 2		2, 3
	Group 2	1.1 ± 1.0	1.1 ± 1.0	1.0 ± 1.0	3.90	0.142			

Note: *p < 0.05; **p < 0.01; Group 1 = Higher functioning group; Group 2 = Lower functioning group; FMA-UE Total score = Fugl-Meyer Assessment-Upper Extremity total score; FMA-UL = Fugl-Meyer Assessment Upper Limb subscore; FMA-Hand = Fugl-Meyer Assessment Hand subscore; WMFT = Wolf Motor Function Test; MAL-AOU = Motor Activity Log - Amount of Use scale (AOU); MAL-QOM = Motor Activity Log - Quality of Movement scale (QOM)

Effects on Hand Functions

Twenty patients with stroke were recruited. There were significant differences among the three times of evaluation – pre-test (1), post-test (2), and three-week follow-up (3) – in FMA-UE Total score (Chi-square = 34.219, p = 0.000), FMA-UL subscore (Chi-square = 31.200, p = 0.000), FMA-Hand subscore (Chi-square = 22.581, p = 0.000), and WMFT (Chi-square = 27.795, p = 0.000). However, there was no significant difference in grip strength among the three evaluations, as shown in Table 2. The TS-VR training did significantly improve affected arm functions. However, it had no significant effect on the grip strength of individuals with stroke.

Post-hoc analysis using Multiple Wilcoxon signed ranks tests with Bonferroni correction ($p \leq 0.05/3$) revealed that there were significant differences (p = 0.000) in (1, 2) of FMA-UE Total score, FMA-UL subscore, FMA-Hand subscore, and WFMT respectively. There were also significant differences (p = 0.000) in (1, 3) of FMA-Total, FMA-UL, FMA-Hand, and WFMT. However, there were no significant differences in (2, 3) of FMA-UE Total score (p = 0.231), FMA-UL subscore (p = 0.536), FMA-Hand subscore (p = 0.076), or WFMT (p = 0.405). The results imply that TS-VR promotes improvements in affected hand functional performance of individuals with stroke after 10 sessions of treatment. There was still a sustaining positive impact on the functioning of individuals' affected hand after the three-week follow up when compared to their baseline performance, and patients also maintained their performance post-training across time.

Effect on Actual Arm use

Actual arm use of the sample of 20 patients was measured using AOU and QOM in the MAL. Significant increases in AOU (Chi-square = 24.618, $p = 0.000$) and QOM (Chi-square = 26.638, $p = 0.000$) in MAL among the three times of evaluations were found using the Friedman test. This finding suggests that TS-AR training encourages more actual arm use of the affected hand in daily life for individuals with chronic stroke, as well as improving their quality of upper-extremity movement.

Further post-hoc analysis using Multiple Wilcoxon signed ranks tests with Bonferroni correction showed that there were significant differences ($p = 0.000$) in (1, 2) and (1, 3) of AOU and QOM respectively. By comparison, there were no significant differences in AOU scores in (2, 3) and QOM scores in (2, 3) ($p = 0.147$ and $p = 0.338$ respectively).

Higher-functioning group and lower-functioning group

To determine which level of severity of upper extremity impairment would benefit more from this treatment, a Friedman Test was used to compare the outcome measures at three times of evaluation in the samples of higher-functioning group and lower-functioning group patients respectively. Both groups showed significant increases in scores at (1), (2), and (3) evaluations among all outcome measures respectively, except for grip strength. In contrast to the lower-functioning group, the higher-functioning group experienced more significant improvements with smaller p -value ($p = 0.000$) in comparisons of outcome measures of FMA-UL, FMA-Hand, FMA-UE Total, and WMFT respectively. Regardless of the significant increases in all upper-extremity outcome measures (except grip strength), the lower-functioning group showed no significant change in multiple comparisons in most of those outcome measures, as reviewed from post-hoc analysis results using Multiple Wilcoxon signed ranks tests with Bonferroni correction. Moreover, there were significant increases of AOU score ($p = 0.000$) and QOM ($p = 0.001$) score in MAL in the higher-functioning group, whereas patients in the lower-functioning group only had a significant increase in their AOU score ($p = 0.002$) among the evaluations.

Discussion

We developed a new and innovative TS-VR training program for the hemiparetic hand after stroke. The main finding of this study was the demonstration of statistically significant improvements in upper-extremity functional movements of patients with hemiparetic stroke after a two-week TS-VR training program. There was statistically significant enhancement in both quality and quantity of the performance of the affected hand during the daily functions of patients. The results of FMA-UE Total, FMA-UL, FMA-Hand, WMFT, MAL-AOU, and MAL-QOM showed significant improvement within groups across the outcome measures among the three measurement occasions. The TS-VR was proved to be useful for training patients' hand function after stroke.

Our study found that the higher-functioning group benefited more from the TS-VR, as indicated in outcome measures of FMA-UL, FMA-Hand, FMA-UE Total, and WMFT respectively, as well as AOU score in MAL. Compared with the higher-functioning group, patients in the lower-functioning group only participated in certain lower levels with limited use of distal joints and muscles with lower speed, whereas

patients in the higher-functioning group could perform a greater variety of movements, with the involvement of greater use of different joints and muscles in upper extremity from proximal to distal, especially hand and isolated finger movement. Moreover, the nature of our TS-VR training is duration-fixed (30 minutes) but not repetitive or interval-fixed. Patients in the higher-functioning group were able to perform higher repetitions because of their faster rate of performance. This result highlights the significance of the design and nature of TS-VR training in achieving differential benefits to stroke patients with various levels of arm severity. Further research on training duration, repetition, and frequency of the TS-VR program would bring out significance differences in the benefits for higher- and lower- functioning groups.

The significant increase in MAL-QOM score after TS-VR training in the higher-functioning group but not in the lower-functioning group could possibly be explained by their different functional levels. Following completion of the TS-VR program, the overall upper extremity function increased in both groups. However, in the lower-functioning group, the improvement might only be seen in the proximal joint movement (i.e., increased shoulder flexion, external rotation, and elbow extension). The improvements were insufficient for hand functions in the MAL questionnaire, like holding a cup, opening a drawer, or eating with a spoon., Hence, the overall quality of movement in these tasks remained similar after the TS-VR program. The grip strength of both groups showed no significant improvement after the course of TS-VR training. This is understandable as the TS-VR training did not include any strengthening element in any of its levels but only movement control and range of motion.

One of the reasons for the significant improvements after TS-VR training might be attributed to training with high frequency and appropriate intensity. Our treatment program consisted of a total of 10 sessions, each lasting 30 minutes, held five days per week over two consecutive weeks. Previous research has revealed that the intensity of task-specific trainings need not necessarily be high in order to achieve optimal effects. Training sessions that are as short as 15 minutes have resulted in lasting changes in cortical representation [5]. Our findings are consistent with those from numerous previous studies [5–7], which have suggested that less intense (i.e., 30–45 minutes) task-specific training regimens can lead to significant improvements in the use and functions of the affected limb.

We conducted our training on a one-to-one basis with supervised therapy. During each supervised session, the facilitator selected activities that were suitable to the functional level of the patients and determined the repetitions of activities to be performed. Moreover, the facilitator provided specific and ongoing verbal and tactile cues on participants' performance. This extrinsic and instant feedback on movement quality can effectively correct patients' unwanted or compensatory movement patterns, which is also a key principle in skill acquisition [31]. In addition, the 3D and graphically 'enriched' environments with multimodal feedback (visual, auditory, tactile) in VR settings also provided sensory input to the patients, which made them more motivated to attend the training than they would have been to attend conventional training, which is less playful and interactive.

It might also be possible to explain improvements in MAL as resulting from one of the unique features of our VR training program, that is, its adoption of task-specificity in a progressive manner. In order to be 'task specific', each action in the training tasks must specify an object to reach for. The tasks are simulating conditions in real life in order to enhance carry-over into daily life activities (Cunningham et al., 2016). Our TS-VR program is composed of seven functional tasks according to seven ordered levels of increasing complexity. The complexity of the tasks is related to the Brunnstrom theory of development of the hemiparetic upper limb in recovery, with reference to the respective key actions corresponding to levels 1–7 in the FTHUE [21, 22, 30, 31]. Our study, to our knowledge, is the first one incorporating task-specificity with increasing levels of complexity into VR training for the hemiparetic upper extremity. The results may be useful as supporting evidence for integrating task-specificity and virtual reality into programs for the treatment of upper limb motor impairments during stroke rehabilitation.

In our study, we attempted to explore the effectiveness of TS-VR rehabilitation that focused on the distal upper extremity up to the forearm, using the LMC as an input device. The advantage of the LMC is that it is cheap and easily set up, requiring only a desktop computer or laptop, the LMC, and our TS-VR training program. There are also existing studies focused more on proximal upper limb rehabilitation [13]. Kinect, which is a widely commercially available motion sensing device, recognizes the body's joint positions, especially for proximal joints like shoulder and elbow. However, VR systems like Kinect do not benefit the distal joints, which are important in hand function training such as grasp and release. To address this limitation, we used the LMC in our TS-VR program, as this motion sensor is able to capture the motion of wrist and of each of the finger joints, enabling it to accurately measure fine motor movements [15]. To further develop our TS-VR program in the future, we suggest combining the use of Kinect and the LMC, as there are currently no VR systems involving both proximal and distal upper extremity movements at the same time [32]. Further research to explore the effectiveness of the combined use of devices that can measure both gross motor and fine motor abilities would be useful is recommended as a direction for future investigations.

Conclusions

This study showed that our newly designed TS-VR training system was useful and led to significant improvements in the upper extremity functions of patients with chronic hemiparetic stroke after a 10-session training program. TS-VR is user-friendly and simulates daily hand function tasks, with levels of difficulty customized for different patients, thus motivating them to perform similar tasks in real life. When undertaken with high frequency and at appropriate intensity, it is hoped that this low cost and innovative training program will provide significant benefits to people with stroke in the future.

Abbreviations

AR = augmented reality

FMA-UE Total score = Fugl-Meyer Assessment-Upper Extremity total score

FMA-Hand = Fugl-Meyer Assessment Upper Limb subscore

FMA-Hand = Fugl-Meyer Assessment Hand subscore

FTHUE = Functional Test for the Hemiplegic Upper Extremity

Group 1 = Higher functioning group

Group 2 = Lower functioning group

LMC = Leap Motion controller

MAL-AOU = Motor Activity Log - Amount of Use scale (AOU)

MAL-QOM = Motor Activity Log - Quality of Movement scale (QOM)

TS-VR = task-specific virtual reality program

WMFT = Wolf Motor Function Test

VR = virtual reality

Declarations

Acknowledgements

The authors would like to express their appreciation to the Hong Kong Stroke Association for coordinating the data collection.

Authors' contributions

KNKF designed the study. YMT and KS was responsible for the technical parts, including modeling the virtual content, computer programming, and development of the TS-VR program. KS, AKHY, CCWL, and YWTM were primarily responsible for the data collection, and data analysis. KNKF, YMT, KS, AKHY, CCWL, and YWTM drafted the manuscript. All authors made substantial contributions to the manuscript, and all read and approved the final version.

Funding

The study received no funding from any source.

Availability of data and materials

The datasets generated during and/or analyzed during the current study are available from the corresponding authors on reasonable request.

Ethics approval and consent to participate

Written and informed consent was obtained from all patients before the study commenced. The study was carried out in accordance with the principles of the Declaration of Helsinki. Ethical approval was sought and obtained from the Human Ethics Committee of the Hong Kong Polytechnic University (HSEARS20180503002).

Competing for publication

All patients gave their written informed consent to participate in this study.

Competing interests

The authors declare that they have no competing interests with respect to the research, authorship, and/or publication of this article.

References

1. Dobkin BH. Clinical practice. Rehabilitation after stroke. *New England Journal of Medicine*. 2005;352(16):1677-1684.
2. Kwakkei G, Kollen BJ. Predicting activities after stroke what is clinically relevant?. *International Journal of Stroke*. 2013;8:25-32.
3. Cunningham P, Turton AJ, Van Wijck F, & Van Vliet P. Task-specific reach-to-grasp training after stroke: development and description of a home-based intervention. *Clinical Rehabilitation*. 2016;30(8):731-740.
4. Cauraugh JH & Kim SB. Stroke motor recovery: active neuromuscular stimulation and repetitive practice schedules. *Journal of Neurology, Neurosurgery & Psychiatry*. 2003;74(11):1562-1566.
5. Bayona NA, Bitensky J, Salter K & Teasell R. The role of task-specific training in rehabilitation therapies. *Topics in stroke rehabilitation*. 2005;12(3):58-65.
6. Galea MP, Miller KJ, & Kilbreath SL. Early task-related training enhances upper limb function following stroke. Poster presentation (March 25 – 30, 2001) at the annual meeting of the Society for Neural Control of Movementvi. Spain: Sevilla; 2001.
7. Page SJ. Intensity versus task-specificity after stroke: how important is intensity?. *American Journal of Physical Medicine & Rehabilitation*. 2003;82(9):730-732.
8. Timmermans AA, Seelen HA, Willmann RD, Rakx W, de Ruyter B, Lanfermann G, & Kingma H. Arm and hand skills: Training preferences after stroke. *Disability and Rehabilitation*. 2009;31:1344-52.
9. Schultheis MT & Rizzo AA. The application of virtual reality technology in rehabilitation. *Rehabilitation Psychology*. 2001;46(3):296.
10. De Mauro A. Virtual reality based rehabilitation and game technology. *Engineering Interactive Computer Systems for Medicine and Healthcare*. 2011;1:48-52.

11. Fong KNK, Chow KKY, Chan BCH, Lam KCK, Lee JCK, Li THY, Yan EWH & Wong AKY. Usability of a virtual reality environment simulating an automated teller machine for assessing and training persons with acquired brain injury. *Journal of NeuroEngineering and Rehabilitation*. 2010;7(19):1-9.
12. Saposnik G, Levin M & Stroke Outcome Research Canada (SORCan) Working Group. Virtual reality in stroke rehabilitation: a meta-analysis and implications for clinicians. *Stroke*. 2011;42(5):1380-1386.
13. Shin JH, Kim MY, Lee JY, et al. Effects of virtual reality-based rehabilitation on distal upper extremity function and health-related quality of life: a single-blinded, randomized controlled trial. *Journal of NeuroEngineering and Rehabilitation*. 2016;13(1):17.
14. Tang YM, Au KMK & Leung Y. Comprehending Products with Mixed Reality (MR): Geometric Relationships and Creativity. *International Journal of Engineering Business Management*. 2018;10:1–12. [DOI:10.1177/1847979018809599]
15. Okazaki S, Muraoka Y, & Suzuki R. Validity and Reliability of Leap Motion Controller for Assessing Grasping and Releasing Finger Movements. *Journal of Ergonomic Technology*. 2017;17(1):32-42.
16. Weichert F, Bachmann D, Rudak B & Fisseler D. Analysis of the Accuracy and Robustness of the Leap Motion Controller. *Sensors*. 2013;13(5):6380-6393.
17. Lee B, Lee D & Chin S. Structural Motion Grammar for Universal Use of LeapMotion: Amusement and Functional Contents Focused. *Journal of Sensors*. 2018;6073786:1-15.
18. Fernández-González P, Carratalá-Tejada M, Monge-Pereira E, et al. Leap motion controlled video game-based therapy for upper limb rehabilitation in patients with Parkinson's disease: a feasibility study. *Journal of NeuroEngineering and Rehabilitation*. 2019;16:133. Available from: <https://doi.org/10.1186/s12984-019-0593-x>
19. Wang ZR, Wang P, Xing L, Mei LP, Zhao J, Zhang T. Leap Motion-based virtual reality training for improving motor functional recovery of upper limbs and neural reorganization in subacute stroke patients. *Neural Regen Res*. 2017;12(11):1823-1831. [DOI:10.4103/1673-5374.219043]
20. Bohannon RW & Smith MB. Interrater reliability of a modified Ashworth scale of muscle spasticity. *Physical Therapy*. 1987;67:206-207.
21. Fong K, Ng B, Chan D, et al. Development of the Hong Kong version of the Functional Test for the Hemiplegic Upper Extremity (FTHUE-HK). *Hong Kong Journal of Occupational Therapy*. 2004;14:21-29.
22. Wilson DJ, Baker LL, & Craddock JA. Functional test for the hemiplegic upper extremity. *American Journal of Occupational Therapy*. 1984;38:159-164.
23. Colgan A. How Does the Leap Motion Controller Work?. Leap Motion Blog. 2017 Jan 18. Available from: blog.leapmotion.com/hardware-to-software-how-does-the-leap-motion-controller-work/.
24. Krastev G & Andreeva M. A Software Tool for Experimental Study Leap Motion. *International Journal of Computer Science & Information Technology*. 2015;7(6):145-153.
25. Duncan PW, Propst M & Nelson SG. Reliability of the Fugl-Meyer assessment of sensorimotor recovery following cerebrovascular accident. *Physical Therapy*. 1983;63(10):1606-1610.

26. Fugl-Meyer AR & Jaasko L. Post-stroke hemiplegia and ADL performance. *Scandinavian Journal of Rehabilitation Medicine*. 1980;7:140-152.
27. Wolf SL, Thompson PA, Morris DM, Rose DK, Winstein CJ, Taub E, et al. The EXCITE trial attributes of the Wolf Motor Function Test in patients with subacute stroke. *Neurorehabilitation and Neural Repair*. 2005;19:194-205.
28. Fugl-Meyer AR, Jääskö L, Leyman I, Olsson S, Steglind S. The post-stroke hemiplegic patient. 1. a method for evaluation of physical performance. *Scand J Rehabil Med*. 1975;7(1):13-31.
29. Ng AKY, Leung DPK & Fong KNK. Clinical utility of the Action Research Arm Test, Wolf Motor Function Test and the Motor Activity Log of hemiparetic upper extremity functions after stroke: a pilot study. *Hong Kong Journal of Occupational Therapy*. 2008;18(1):20-27.
30. Uswatte G, Taub E, Morris D, Light K & Thompson PA. The Motor Activity Log-28: assessing daily use of the hemiparetic arm after stroke. *Neurology*. 2006;67:1189-1194.
31. Magill RA & Anderson DI. *Motor learning and control: Concepts and applications (Vol. 11)*. New York: McGraw-Hill; 2007.
32. Seo NJ, Kumar JA, Hur P, Crocher V, Motawar B & Lakshminarayanan K. Usability evaluation of low-cost virtual reality hand and arm rehabilitation games. *Journal of Rehabilitation Research and Development*. 2016;53(3):321-334.

Figures

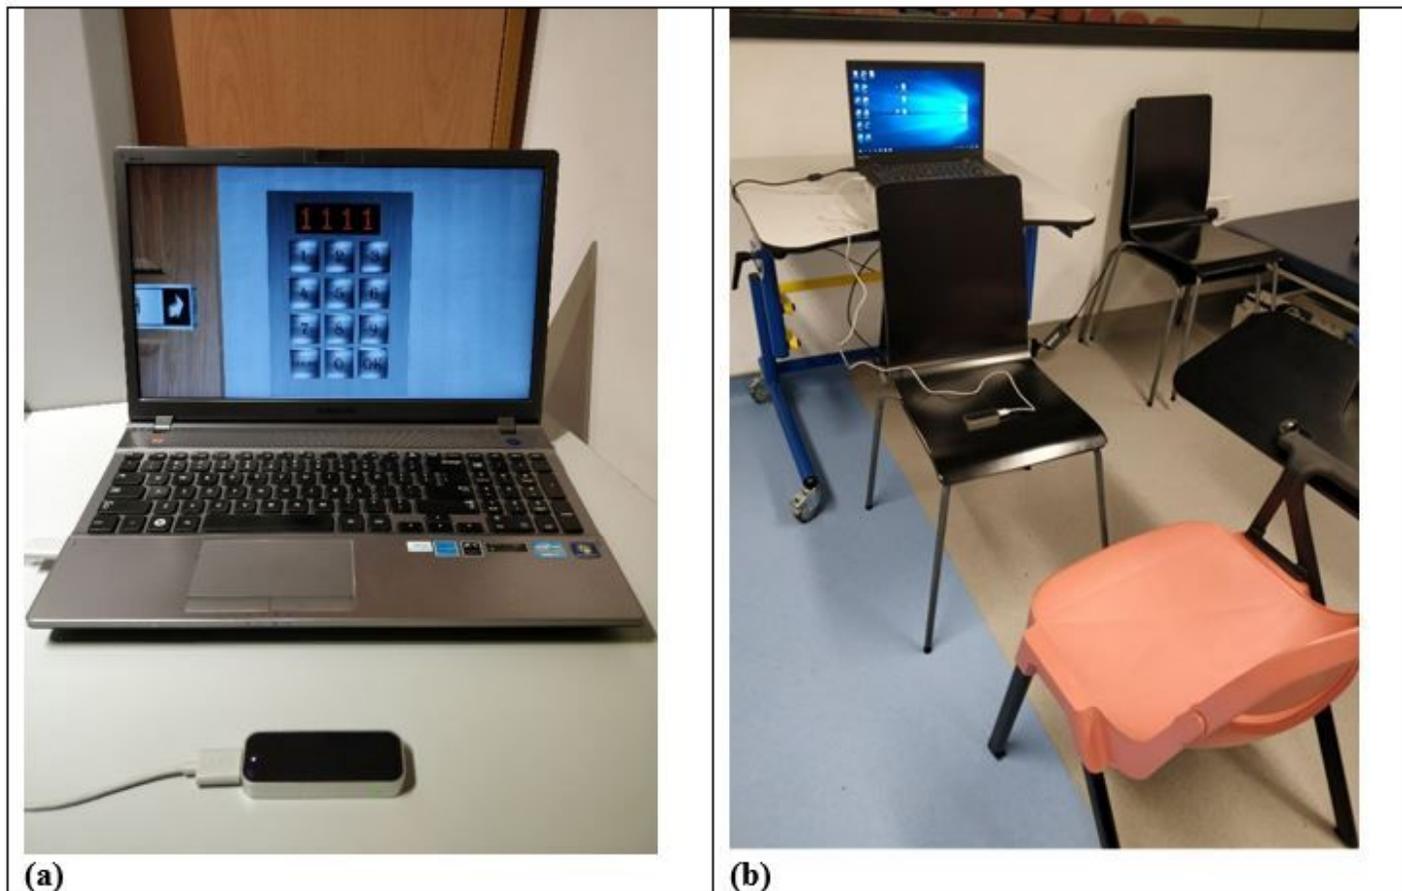


Figure 1

The experimental setup. Figure 1a. The Leap Motion Controller used to capture the motion of the wrist and each finger joint. Figure 1b. Setup of the experiment. The LMC was installed in front of the monitor. The patients were seated in front of the computer and provided with enough space for them to move the upper extremity in order to complete the TS-VR tasks.

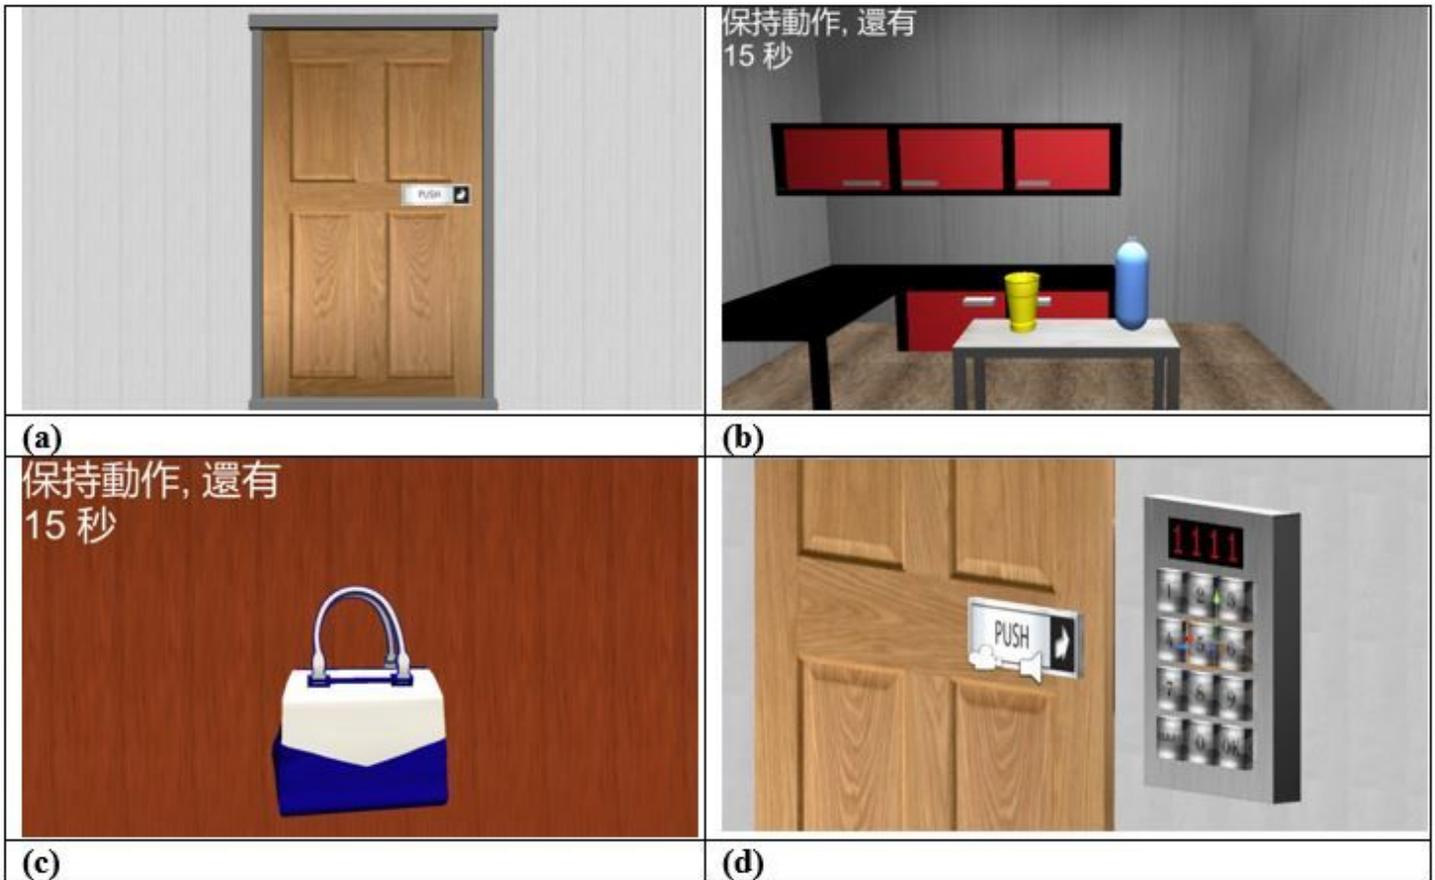


Figure 2

Samples of the TS-VR training task. Figure 2a. Task 1 - Pushing Door; Figure 2b. Task 5 - Pour water from the bottle; Figure 2c. Task 3 - Hold pouch for 15 seconds; Figure 2d. Task 7 – Pressing password pad.

```

Password = generatePassword ();
FindGameObject()
Foreach (GameObject) {
    if (GameObject == Password Pad) {
        switch (trigger_collider) {
            case "INPUT1":
                input[0] = GameObject.digit;
                continue;
            case "INPUT2":
                input[1] = GameObject.digit;
                continue;
            case "INPUT3":
                input[2] = GameObject.digit;
                continue;
            case "INPUT4":
                input[3] = GameObject.digit;
                continue;
        }
    }
}

if (input == password) {
    input [0].text = "D";
    input [1].text = "O";
    input [2].text = "N";
    input [3].text = "E";
    FinishGame();
}
else {
    input [0].text = "F";
    input [1].text = "A";
    input [2].text = "I";
    input [3].text = "L";
    RestartGame();
}

```

Figure 3

Example of pseudo code of the pressing password task. Pseudo code of the pressing password task in Figure 2(d) - The program starts by generating a 4-digit random password. All game objects in the virtual scenes will be searched. If the game object is a password pad and the collider is triggered, then the corresponding digits of the input number will be saved. Finally, the input number will be checked to see if it matches with the random password. The task will end if the password is matched; otherwise, the task will restart.